

SUPERVISOR TEST

CFO
LATIC




ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906

Date: 01/15/2020

OPERATOR NAME:
EMRAH LATIC
Permit #: 46908
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	20:17
INTERNAL STANDARD	VERIFIED	20:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	20:17
BLANK TEST	0.00	20:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	20:19
BLANK TEST	0.00	20:19
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	20:20
BLANK TEST	0.00	20:21

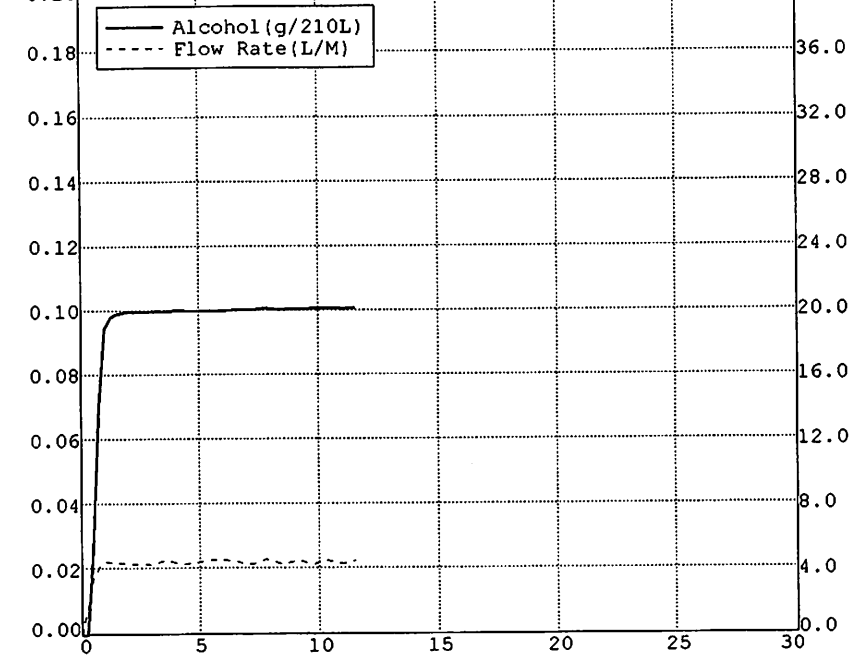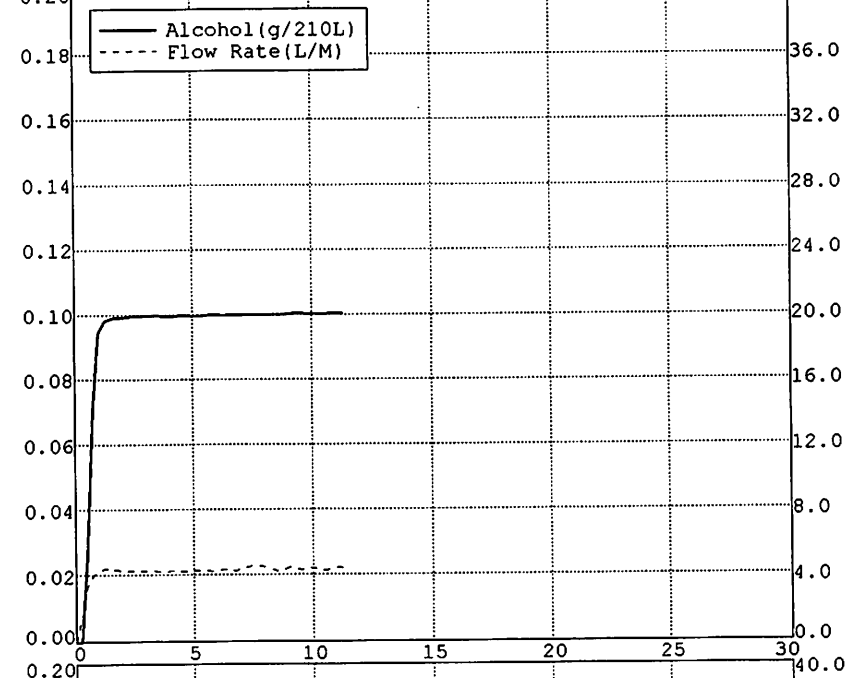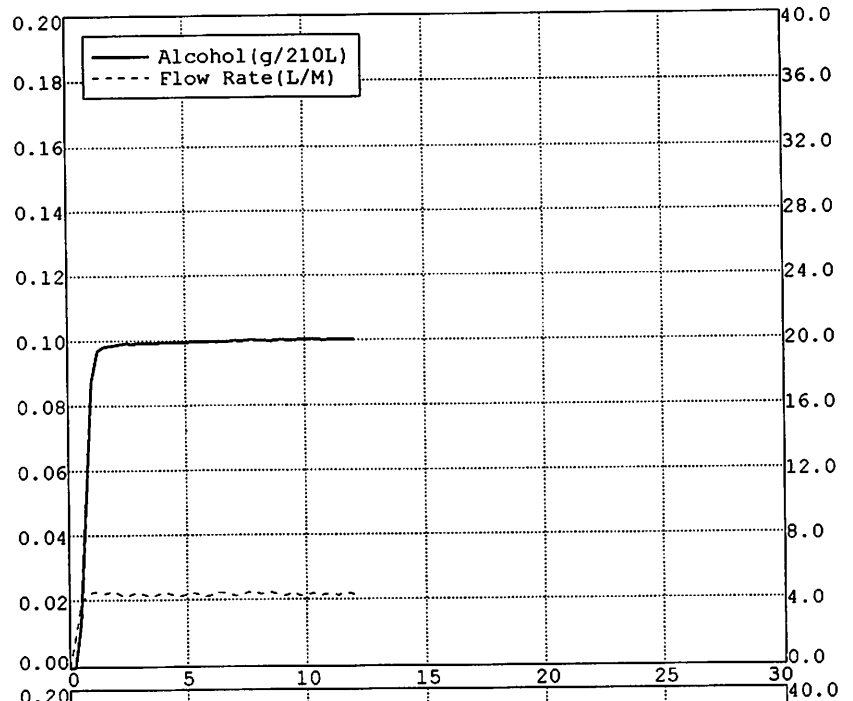

SUPERVISOR TEST

CFO

ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906

Date: 01/22/2020

OPERATOR NAME:
BRETT A GRABELDINGER
Permit #: 46896
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:31
INTERNAL STANDARD	VERIFIED	21:31
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:32
BLANK TEST	0.00	21:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:33
BLANK TEST	0.00	21:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:34
BLANK TEST	0.00	21:35

