

SUPERVISOR TEST

CFD

ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906




Lanc

Date: 03/03/2020

OPERATOR NAME:
EMRAH LATIC
Permit #: 46908
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:38
INTERNAL STANDARD	VERIFIED	02:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.08	02:39
BLANK TEST	0.00	02:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.08	02:40
BLANK TEST	0.00	02:41
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.08	02:42
BLANK TEST	0.00	02:43

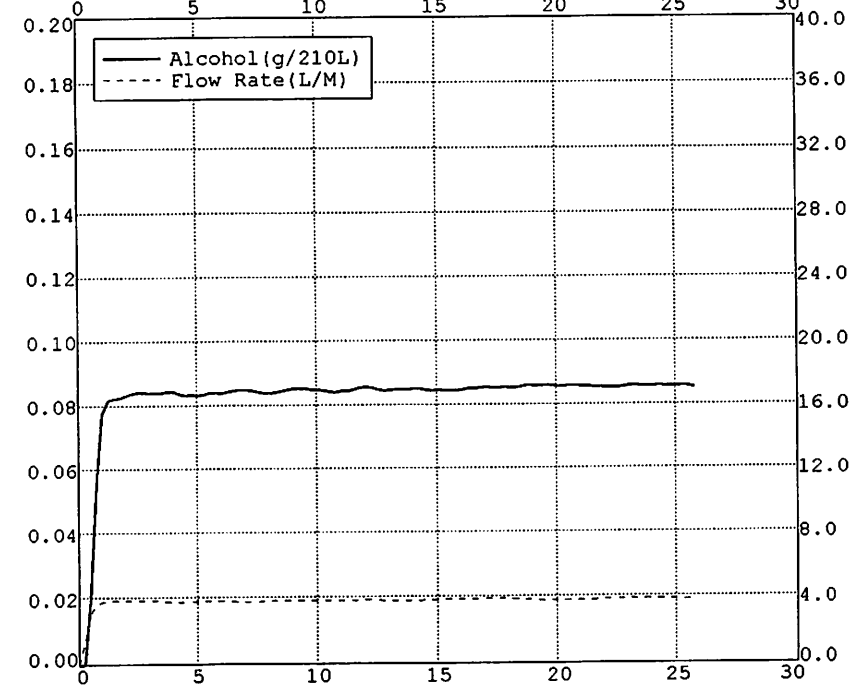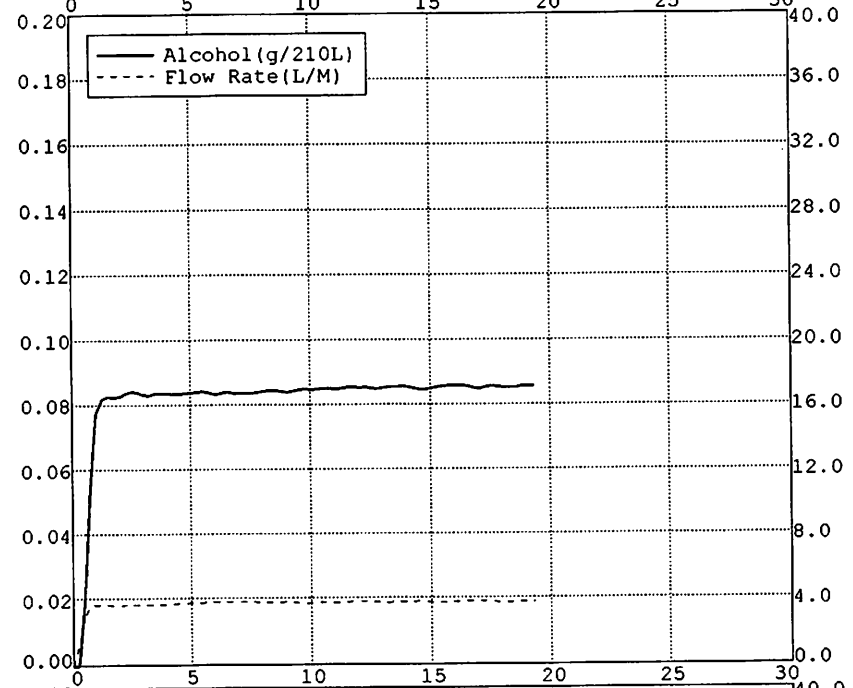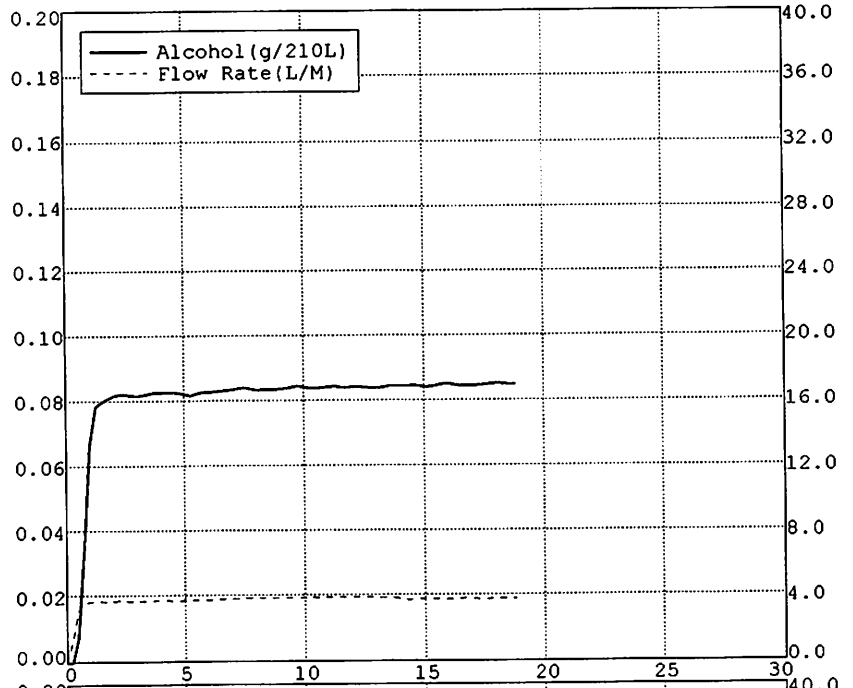

SUPERVISOR TEST

ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906




CFO

Date: 03/04/2020

OPERATOR NAME:
JASON L OSIKA
Permit #: 35567
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:09
INTERNAL STANDARD	VERIFIED	22:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.07	22:10
BLANK TEST	0.00	22:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.07	22:11
BLANK TEST	0.00	22:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.07	22:12
BLANK TEST	0.00	22:13

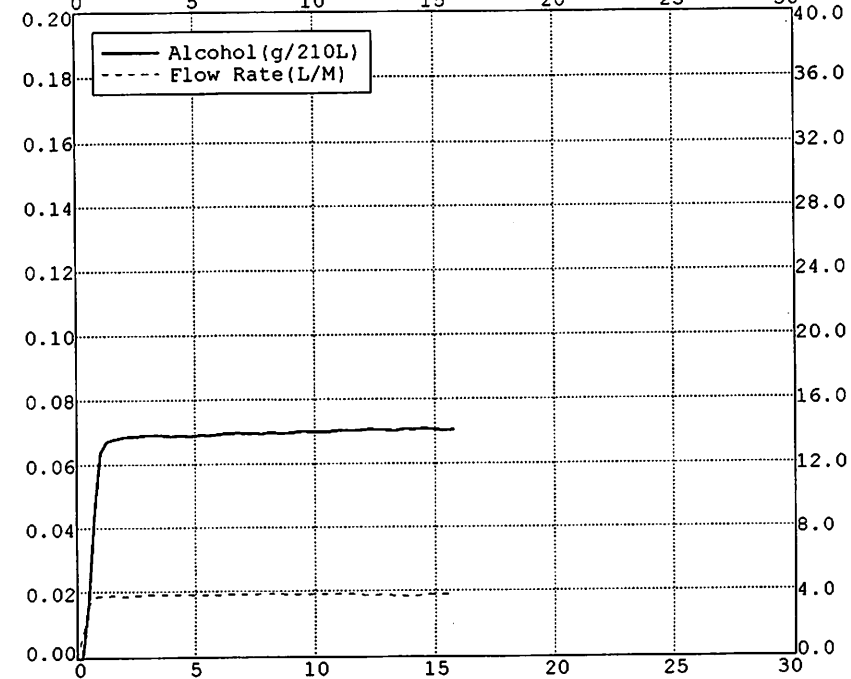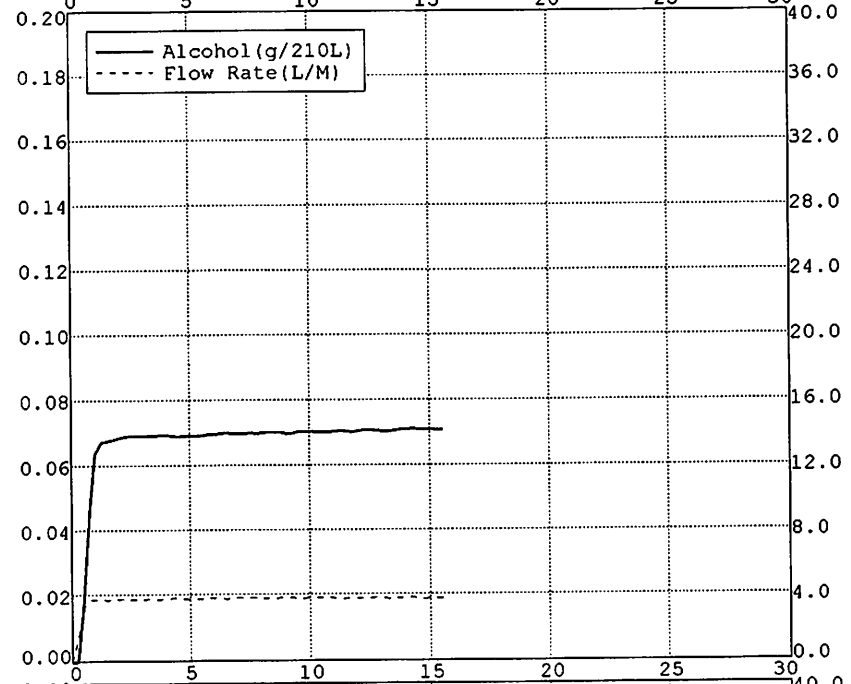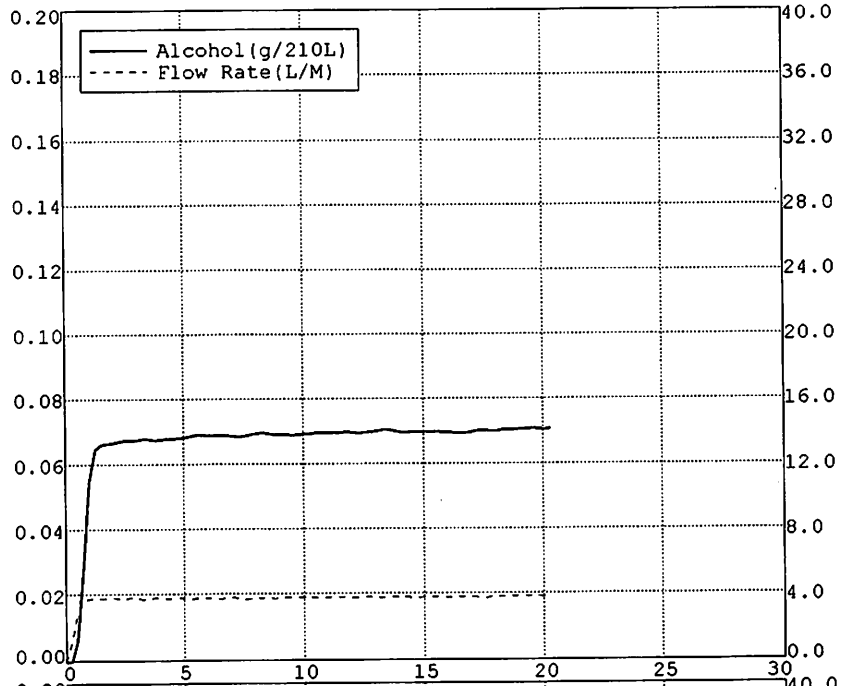

SUPERVISOR TEST

CFO

LATIC

ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906

Date: 03/11/2020

OPERATOR NAME:
EMRAH LATIC
Permit #: 46908
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:22
INTERNAL STANDARD	VERIFIED	23:22
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.04	23:22
BLANK TEST	0.00	23:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.04	23:23
BLANK TEST	0.00	23:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.04	23:24
BLANK TEST	0.00	23:25

