

SUPERVISOR TEST

ONEIDA CO.  
SHERIFF'S DEPT  
DATAMASTER dmt: 123906



Date: 04/22/2020

OPERATOR NAME:  
BRANDON J RUTLEDGE  
Permit #: 43762  
Operator Agency/Dept: ONEIDA CO. SO  
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:31
INTERNAL STANDARD	VERIFIED	22:31
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	22:31
BLANK TEST	0.00	22:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	22:33
BLANK TEST	0.00	22:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	22:34
BLANK TEST	0.00	22:35

*CFO*

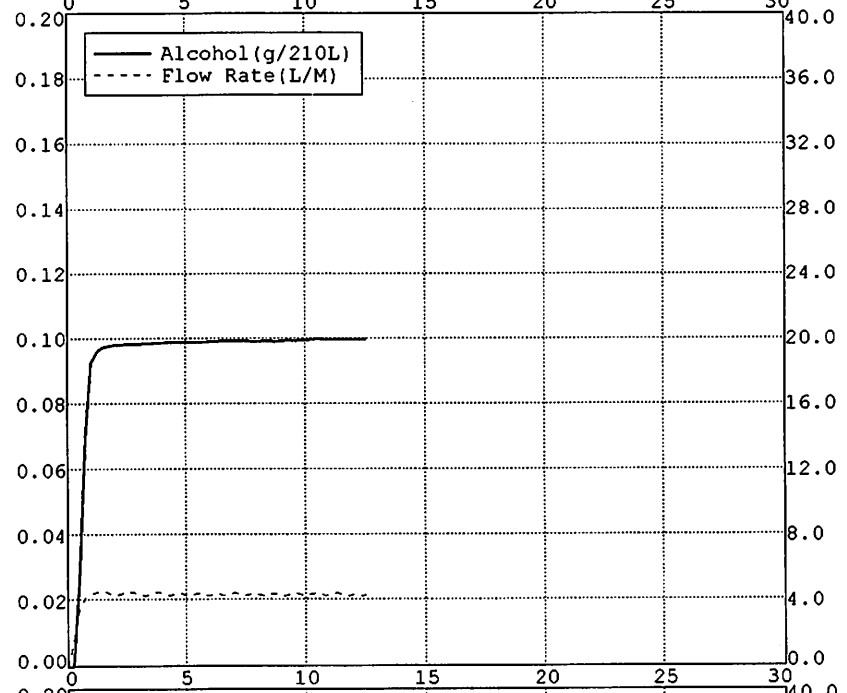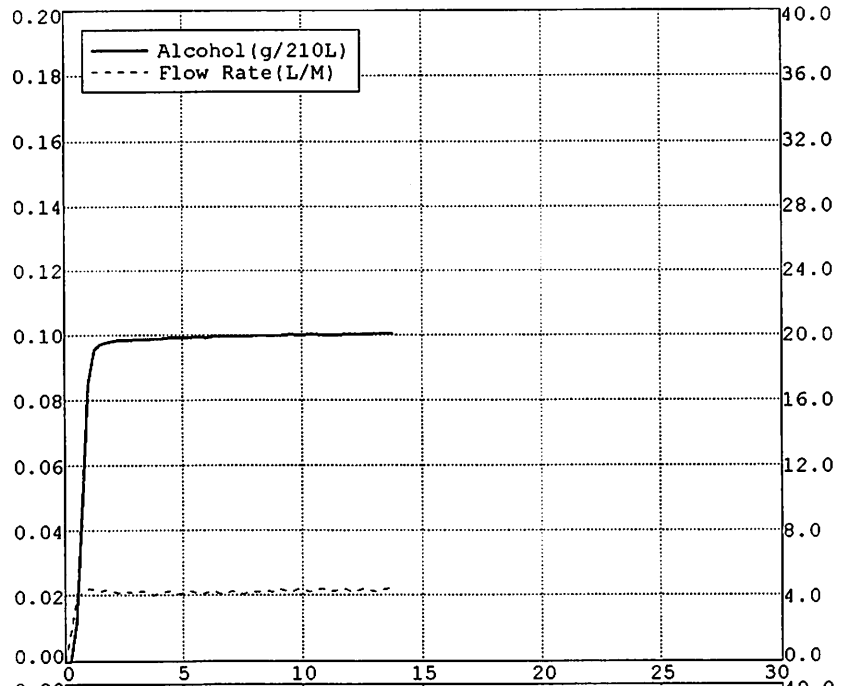

SUPERVISOR TEST

CFO




ONEIDA CO.  
SHERIFF'S DEPT  
DATAMASTER dmt: 123906

Date: 04/29/2020

OPERATOR NAME:  
BRETT A GRABELDINGER  
Permit #: 46896  
Operator Agency/Dept: ONEIDA CO. SO  
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	20:43
INTERNAL STANDARD	VERIFIED	20:43
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	20:43
BLANK TEST	0.00	20:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	20:44
BLANK TEST	0.00	20:45
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	20:45
BLANK TEST	0.00	20:46

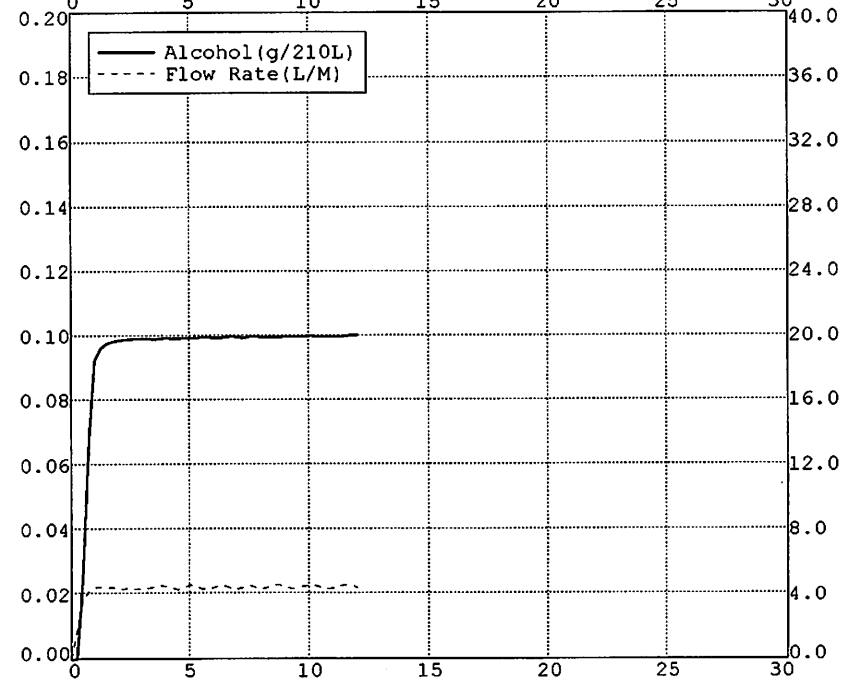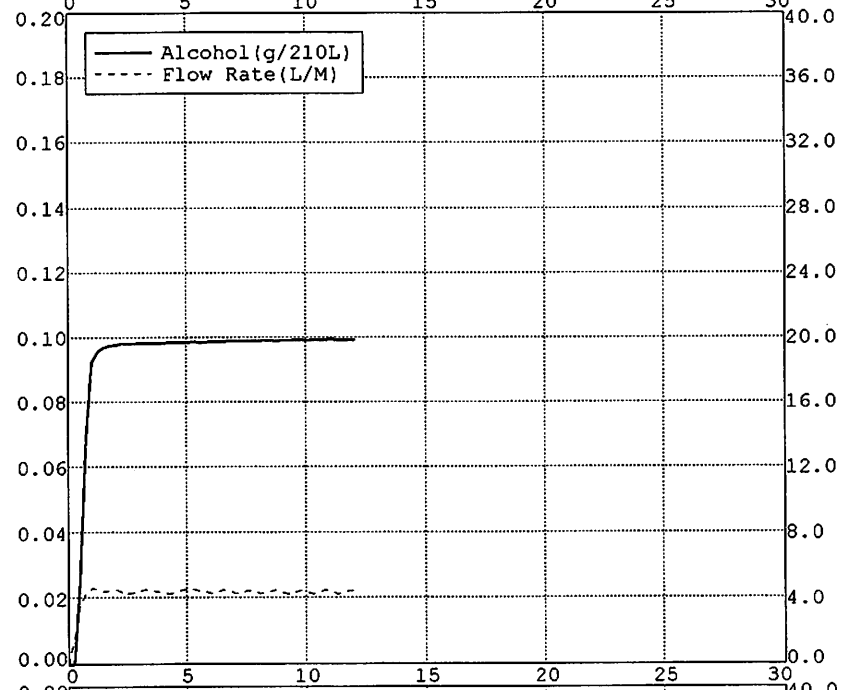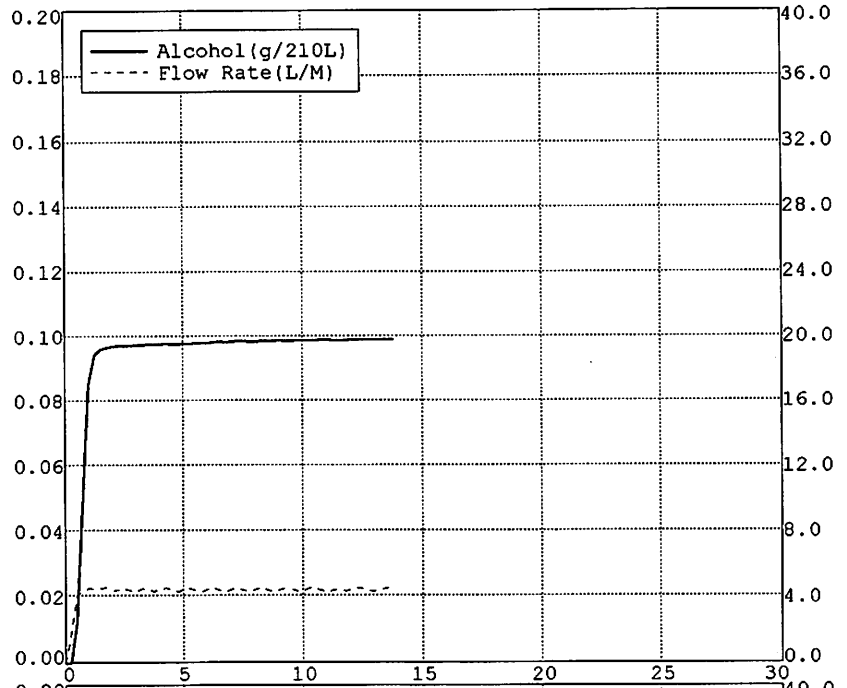

SUPERVISOR TEST

CFO

ONEIDA CO.  
SHERIFF'S DEPT  
DATAMASTER dmt: 123906

Date: 05/05/2020

OPERATOR NAME:  
BRETT A GRABELDINGER  
Permit #: 46896  
Operator Agency/Dept: ONEIDA CO. SO  
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:32
INTERNAL STANDARD	VERIFIED	00:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:33
BLANK TEST	0.00	00:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:34
BLANK TEST	0.00	00:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:35
BLANK TEST	0.00	00:36

