

SOLUTION CHANGE




ROME CITY
 POLICE DEPT
 DATAMASTER dmt: 106106

Date: 04/02/2020

OPERATOR NAME:
 HOLLIE B SILVERMAN
 Permit #: 39044
 Operator Agency/Dept: ROME CITY PD
 Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:10
INTERNAL STANDARD	VERIFIED	16:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:10
BLANK TEST	0.00	16:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:11
BLANK TEST	0.00	16:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:13
BLANK TEST	0.00	16:14

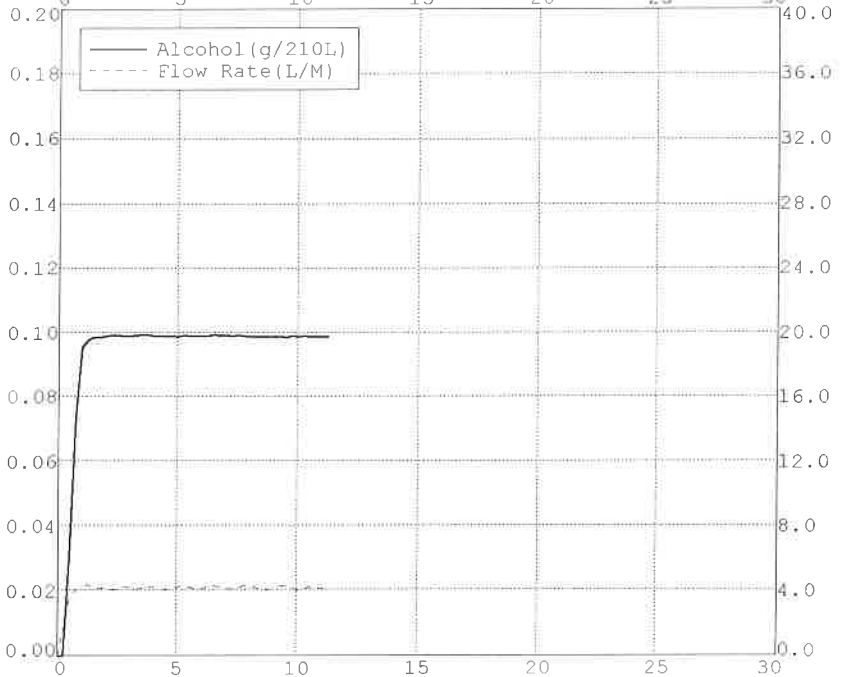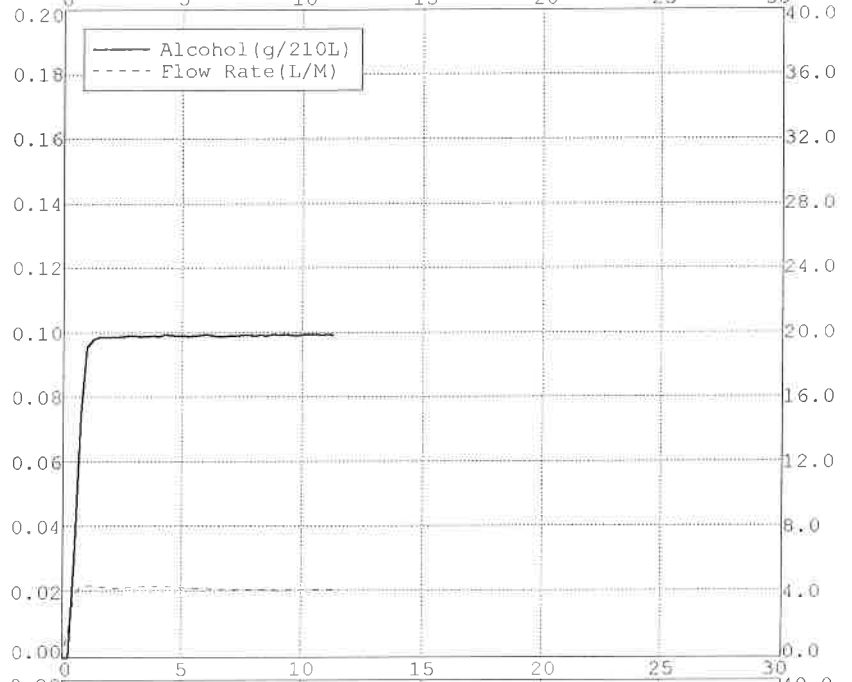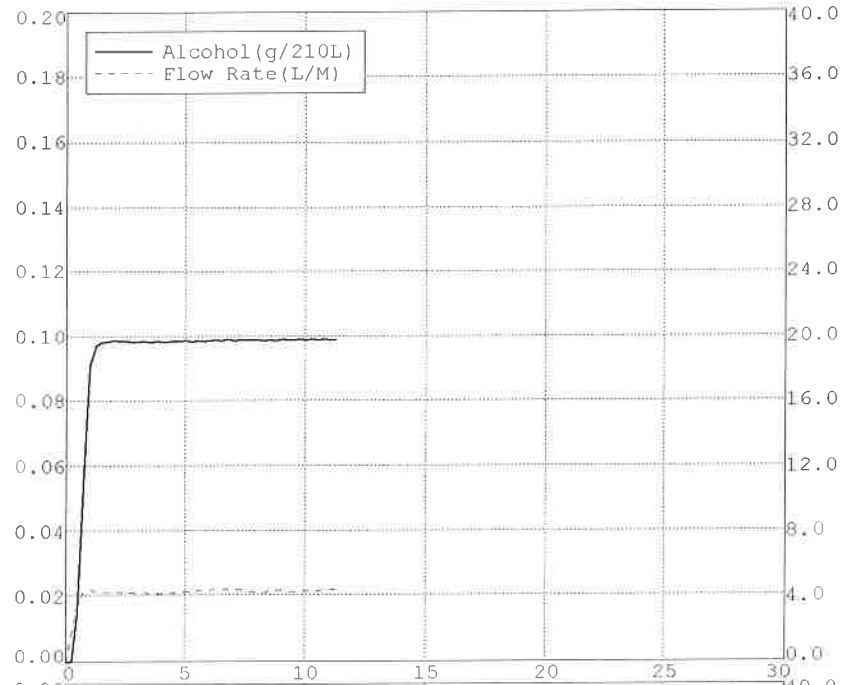

Hollie B Silverman
Rome City PD