

SOLUTION CHANGE



ROME CITY
 POLICE DEPT
 DATAMASTER dmt: 106106

Date: 12/02/2019

OPERATOR NAME:
 HOLLIE B SILVERMANH
 Permit #: 39044
 Operator Agency/Dept: ROME CITY PD
 Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:10
INTERNAL STANDARD	VERIFIED	16:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:11
BLANK TEST	0.00	16:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:12
BLANK TEST	0.00	16:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:13
BLANK TEST	0.00	16:14

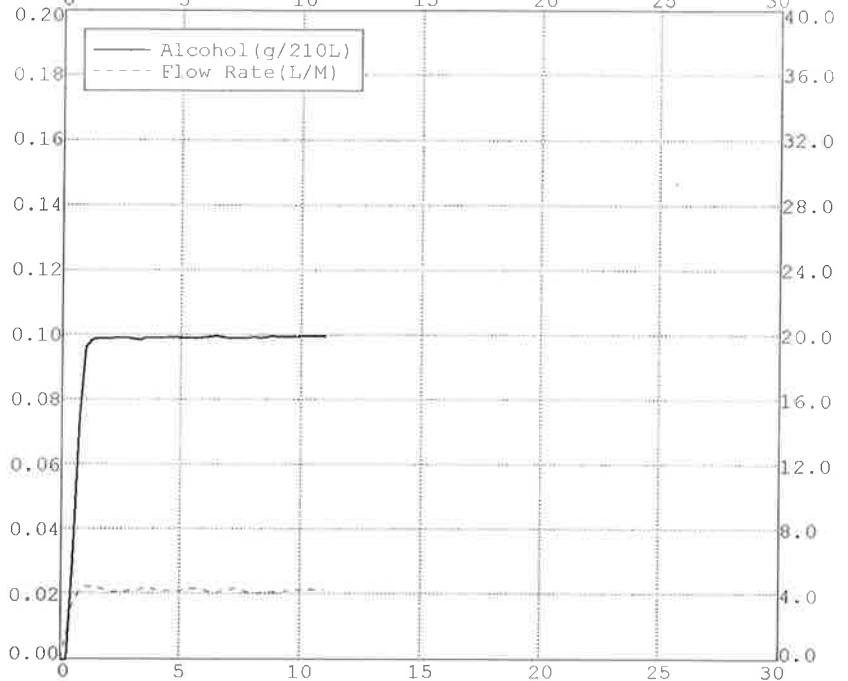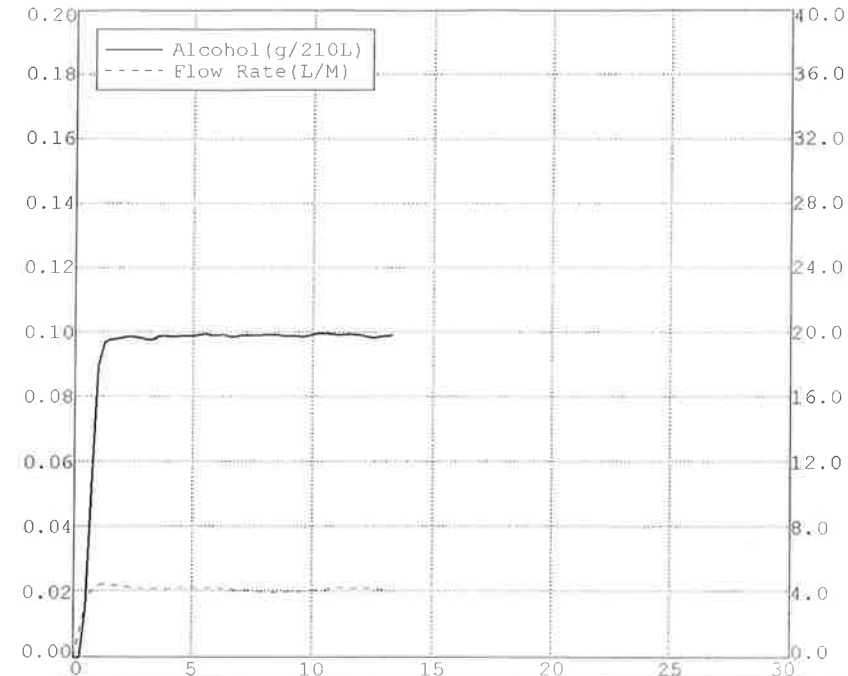

Hollie B Silverman Rome PD 12/02/19
Hollie B. Silverman 106106

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 12/06/2019

OPERATOR NAME:
HOLLIE B SILVERMAN
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:46
INTERNAL STANDARD	VERIFIED	16:46
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:47
BLANK TEST	0.00	16:48
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:48
BLANK TEST	0.00	16:49
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:49
BLANK TEST	0.00	16:50

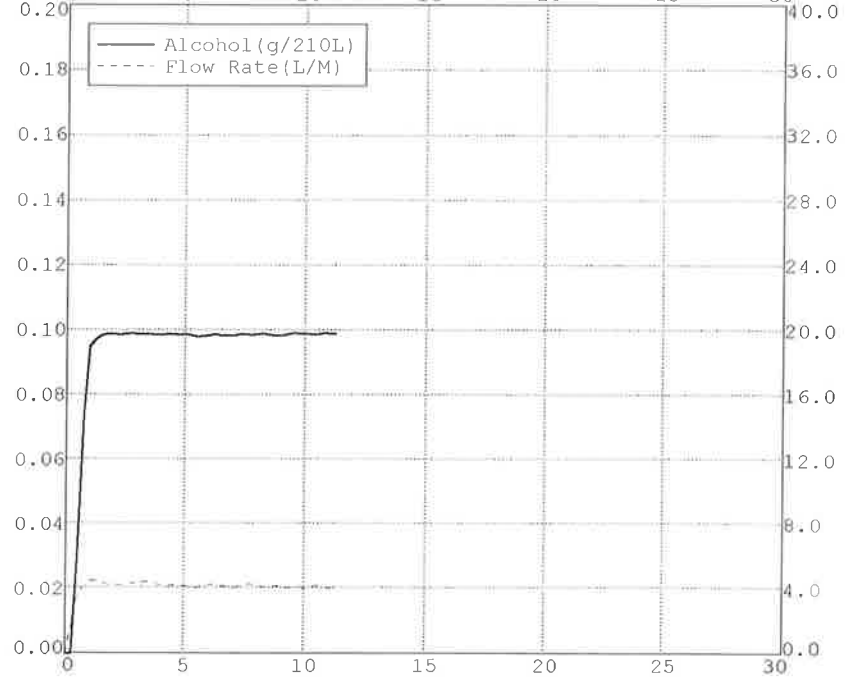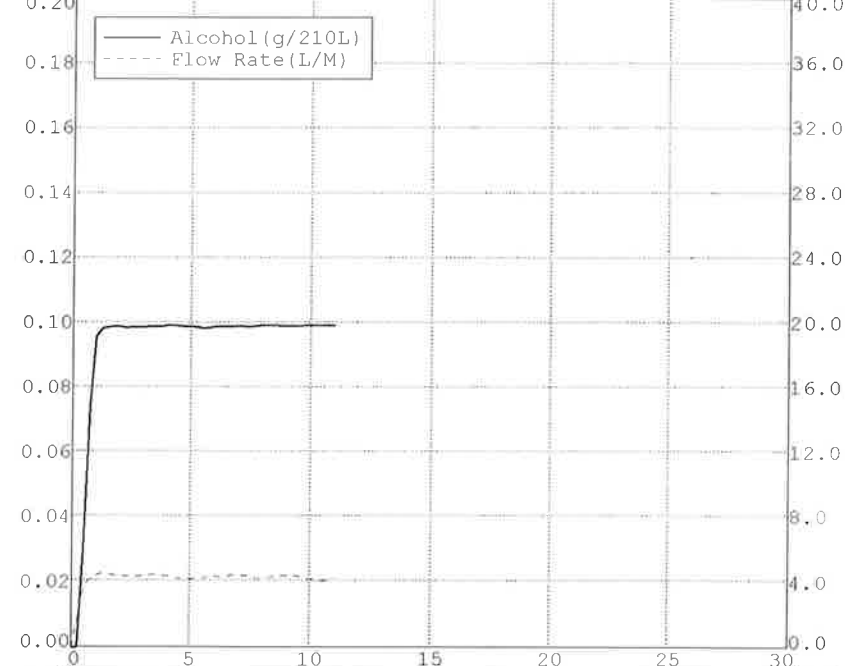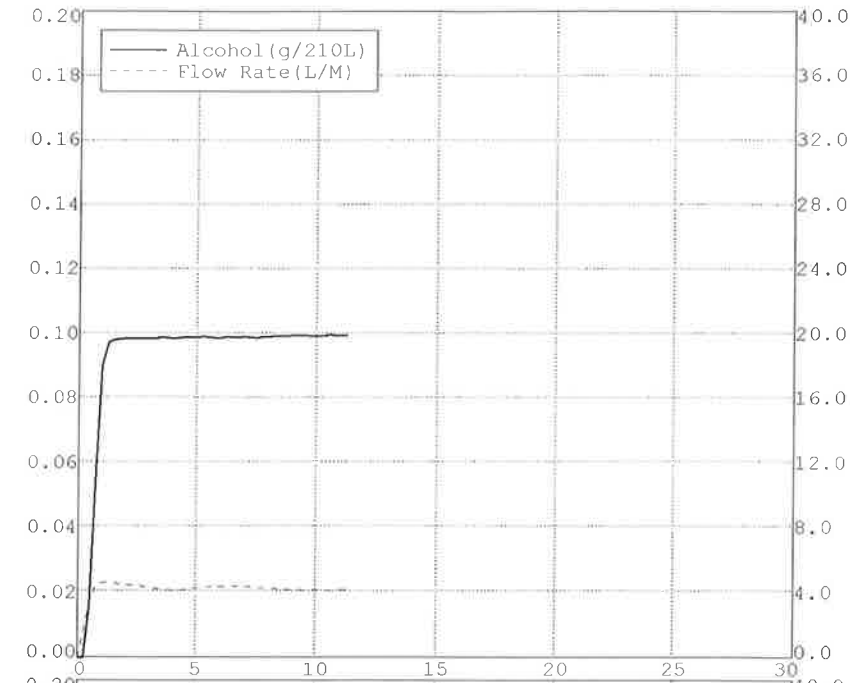

Hollie B Silverman Romepd 12/06/19
Hollie B Silverman 10805

SUPERVISOR TEST




ROME CITY
 POLICE DEPT
 DATAMASTER dmt: 106106

Date: 12/13/2019

OPERATOR NAME:
 HOLLIE B SILVERMAN
 Permit #: 39044
 Operator Agency/Dept: ROME CITY PD
 Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:46
INTERNAL STANDARD	VERIFIED	16:46
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:46
BLANK TEST	0.00	16:47
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:48
BLANK TEST	0.00	16:48
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:49
BLANK TEST	0.00	16:50

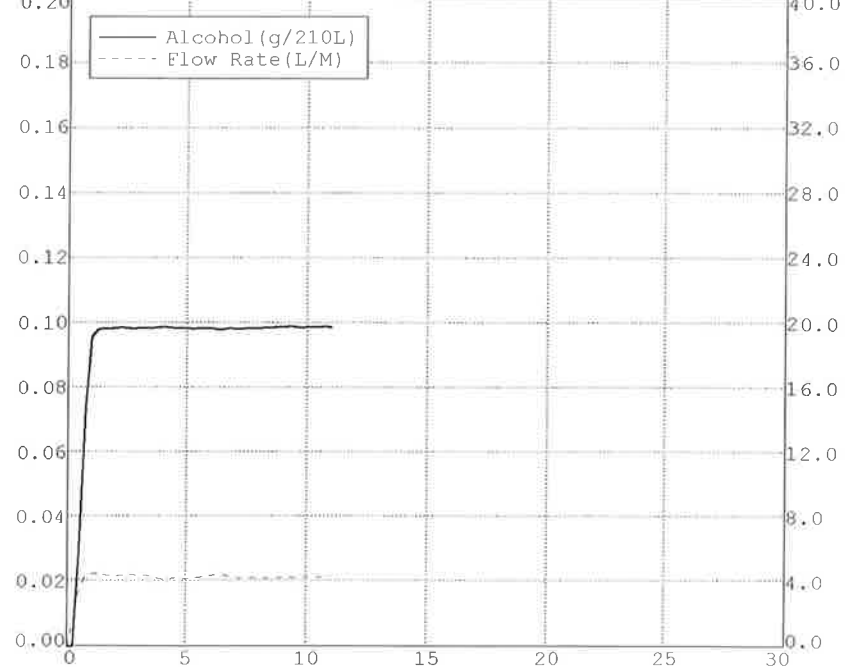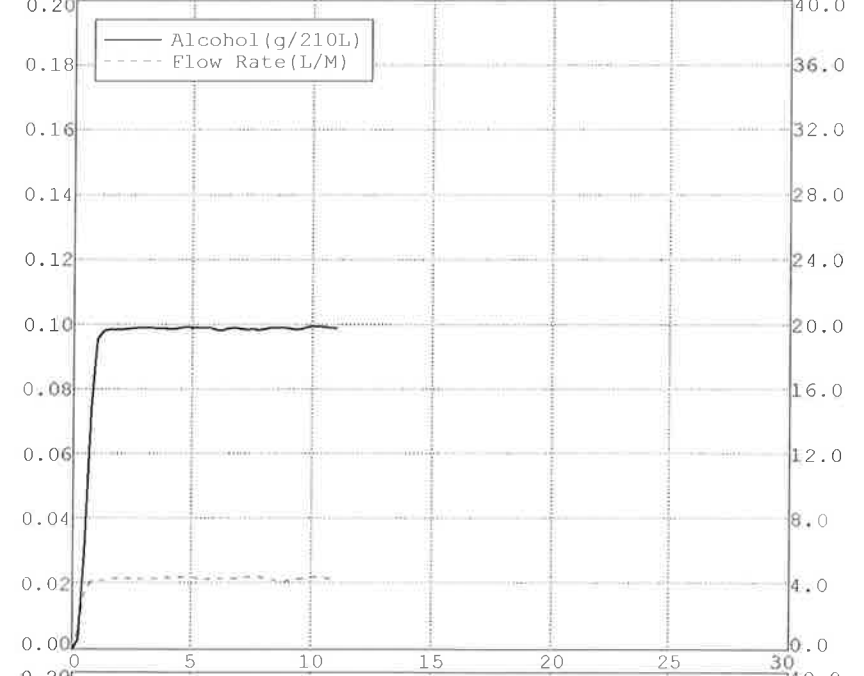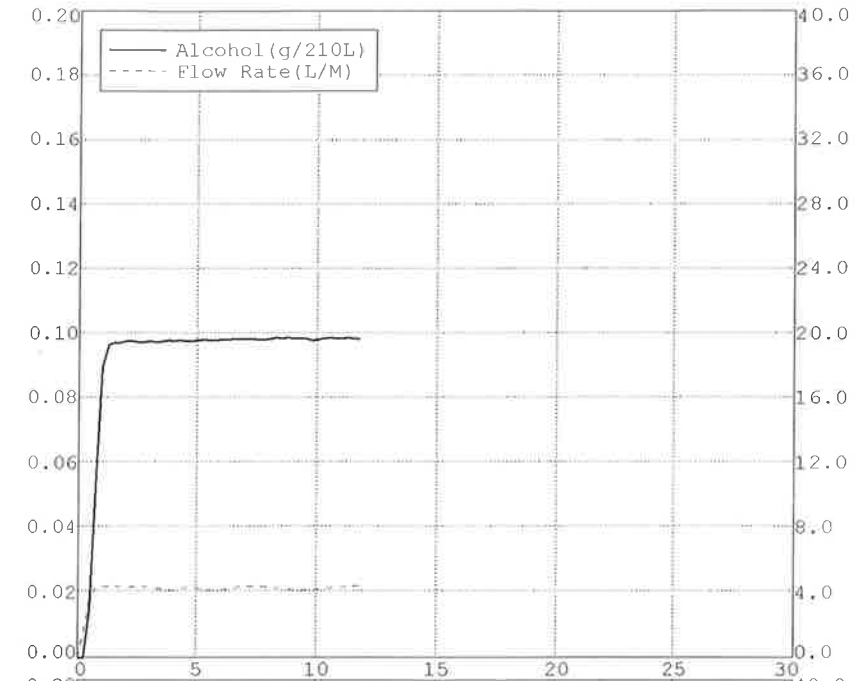

Hollie B. Silverman Rome PD 12/13/19
Hollie B. Silverman 10605

SUPERVISOR TEST




ROME CITY
 POLICE DEPT
 DATAMASTER dmt: 106106

Date: 12/20/2019

OPERATOR NAME:
 HOLLIE B SILVERMAN
 Permit #: 39044
 Operator Agency/Dept: ROME CITY PD
 Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:41
INTERNAL STANDARD	VERIFIED	13:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:42
BLANK TEST	0.00	13:43
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:43
BLANK TEST	0.00	13:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:44
BLANK TEST	0.00	13:45

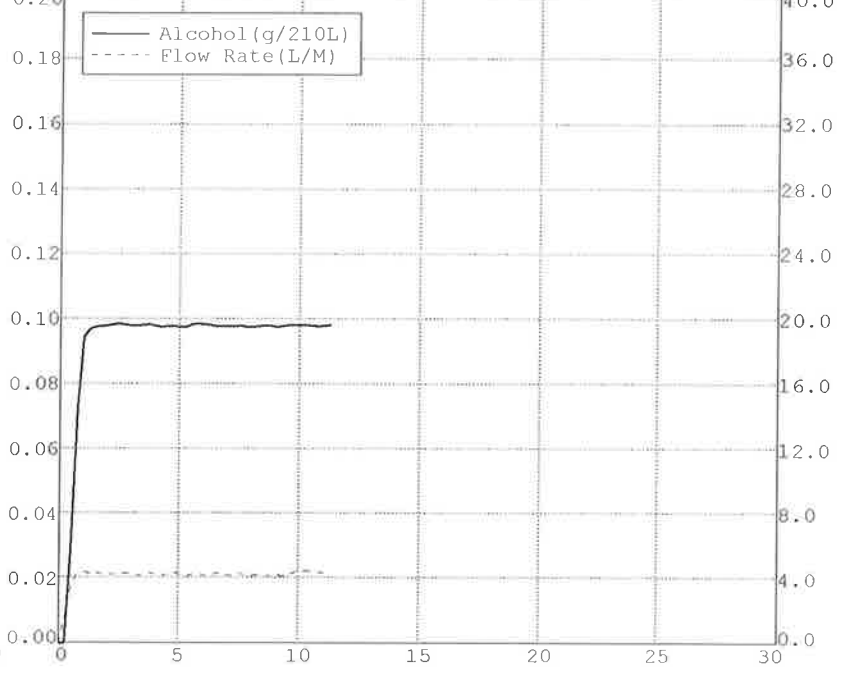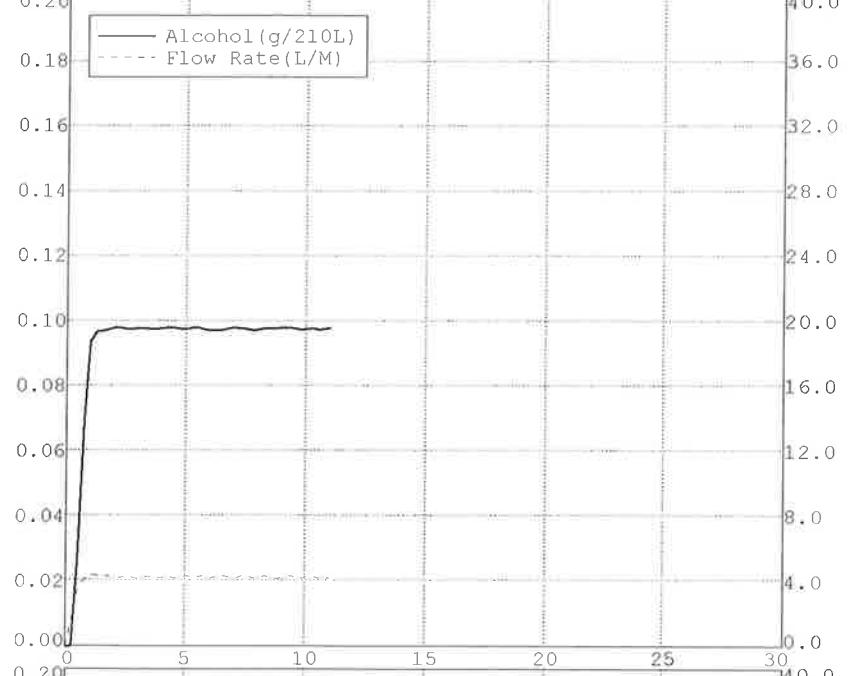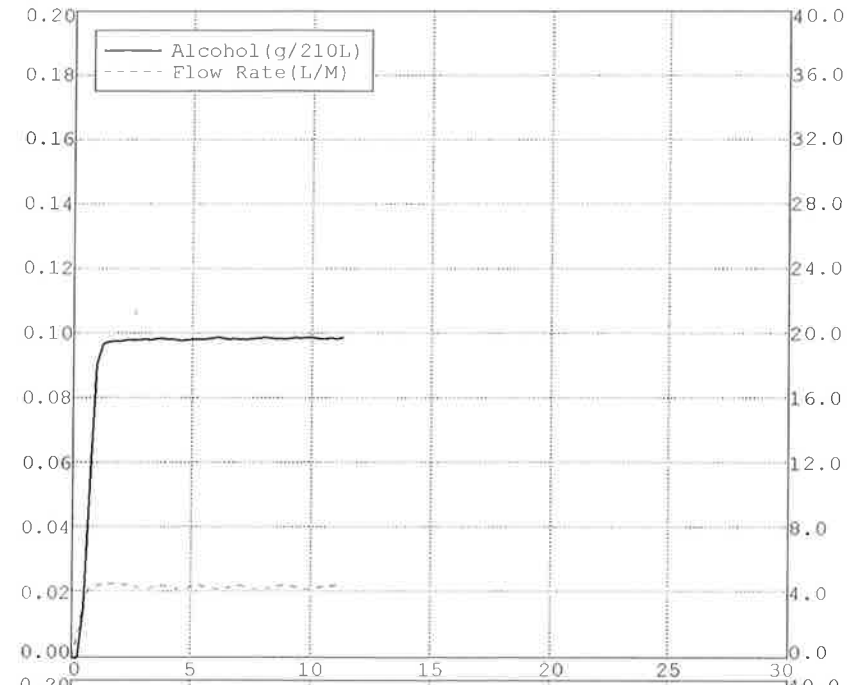

Hollie B Silverman Rome PD 12/20/19
Hollie B Silverman report

SUPERVISOR TEST




ROME CITY
 POLICE DEPT
 DATAMASTER dmt: 106106

Date: 12/28/2019

OPERATOR NAME:
 HOLLIE B SILVERMAN
 Permit #: 39044
 Operator Agency/Dept: ROME CITY PD
 Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:08
INTERNAL STANDARD	VERIFIED	12:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:08
BLANK TEST	0.00	12:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:09
BLANK TEST	0.00	12:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:11
BLANK TEST	0.00	12:12

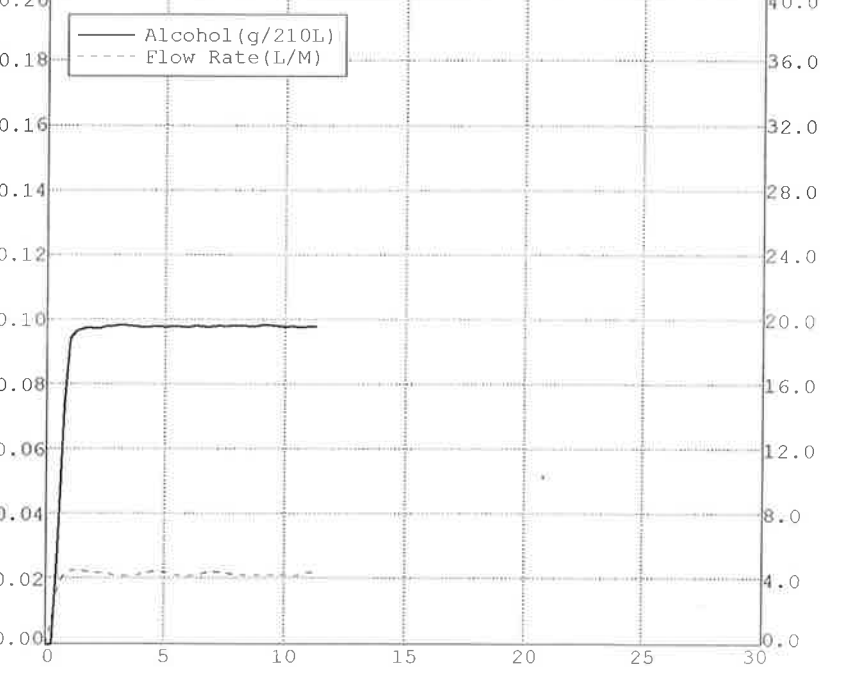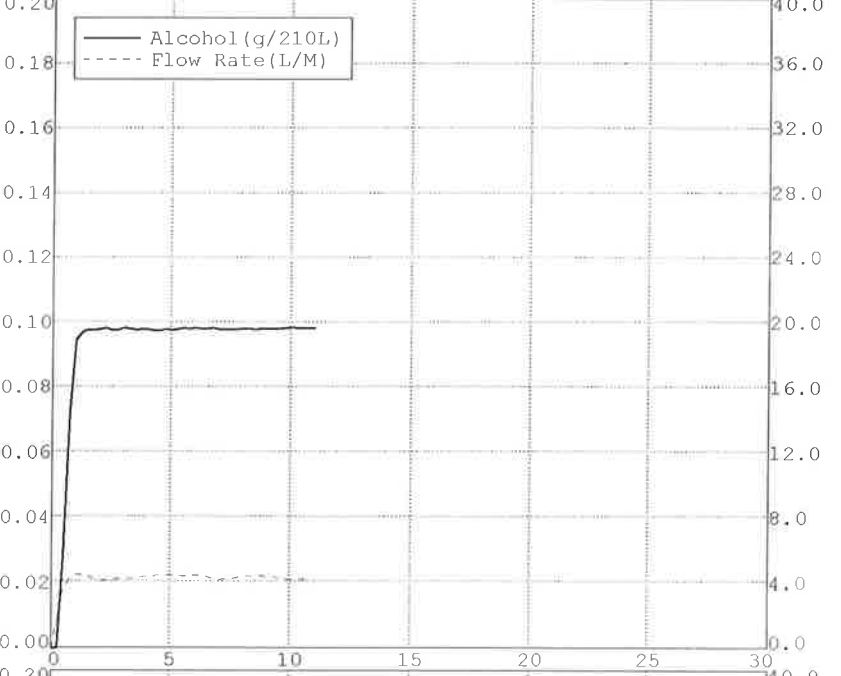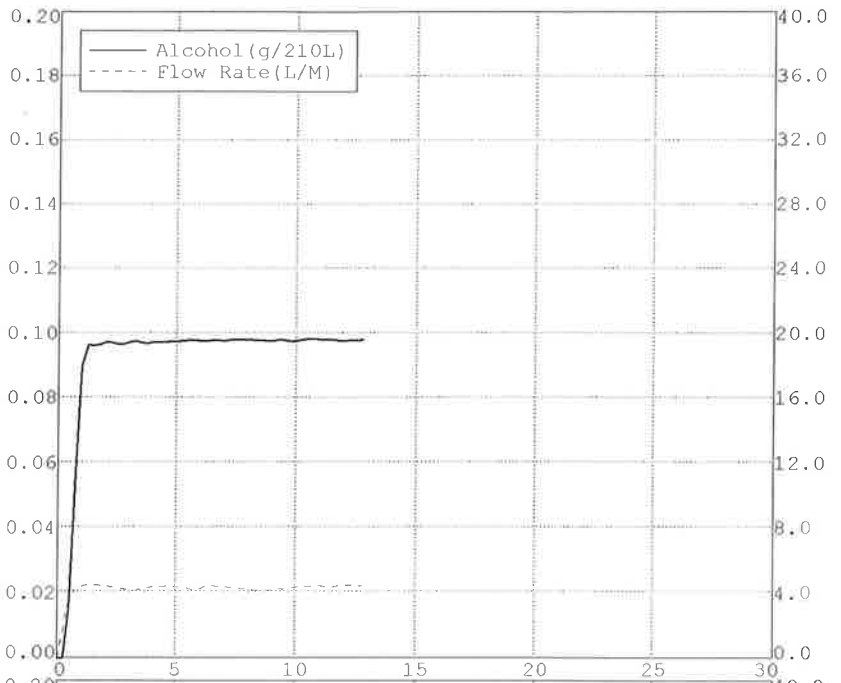

Hollie B. Silverman Rome PD 12/28/19
Hollie B. Silverman 10805