

SOLUTION CHANGE




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 06/02/2019

OPERATOR NAME:
HOLLIE B KENNEDY
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:12
INTERNAL STANDARD	VERIFIED	17:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	17:12
BLANK TEST	0.00	17:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	17:13
BLANK TEST	0.00	17:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	17:14
BLANK TEST	0.00	17:15

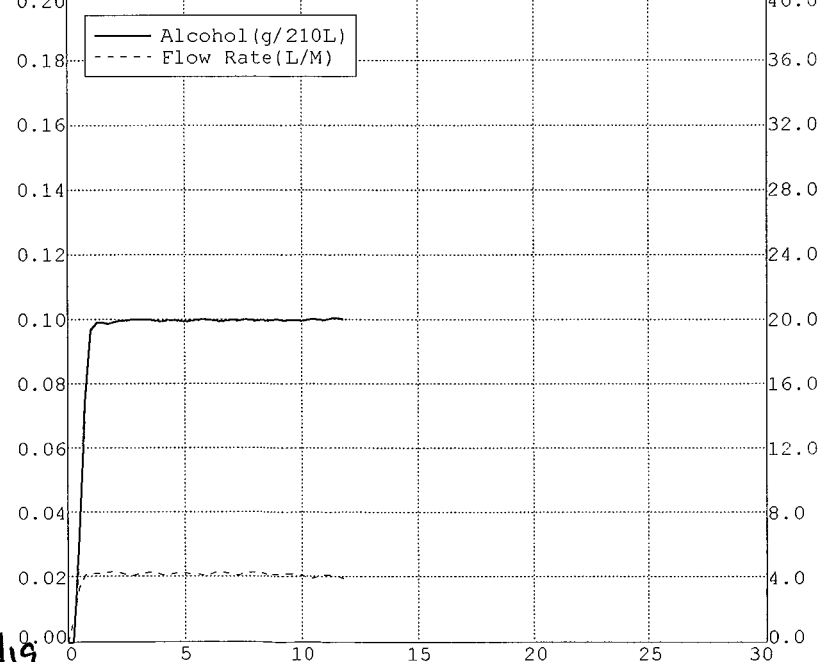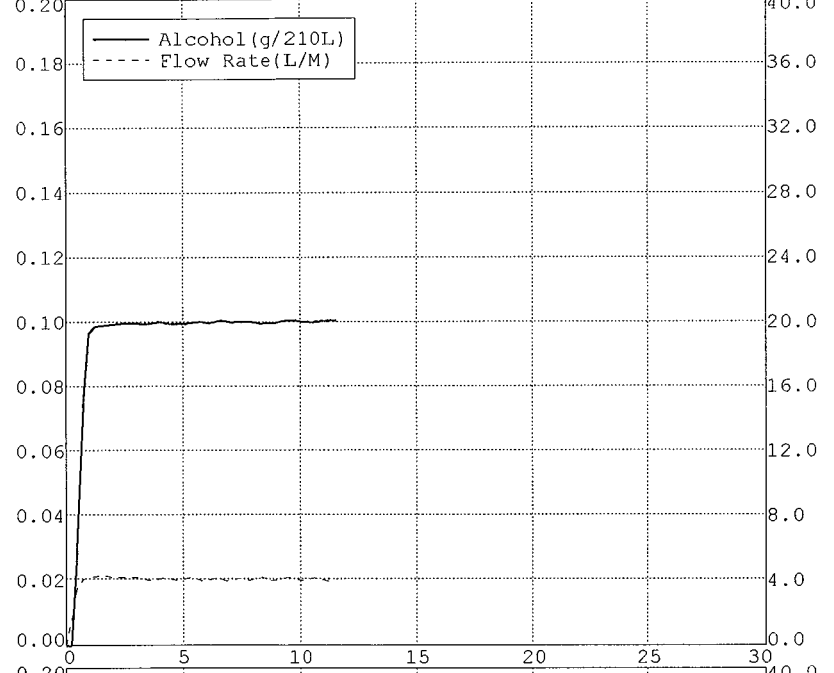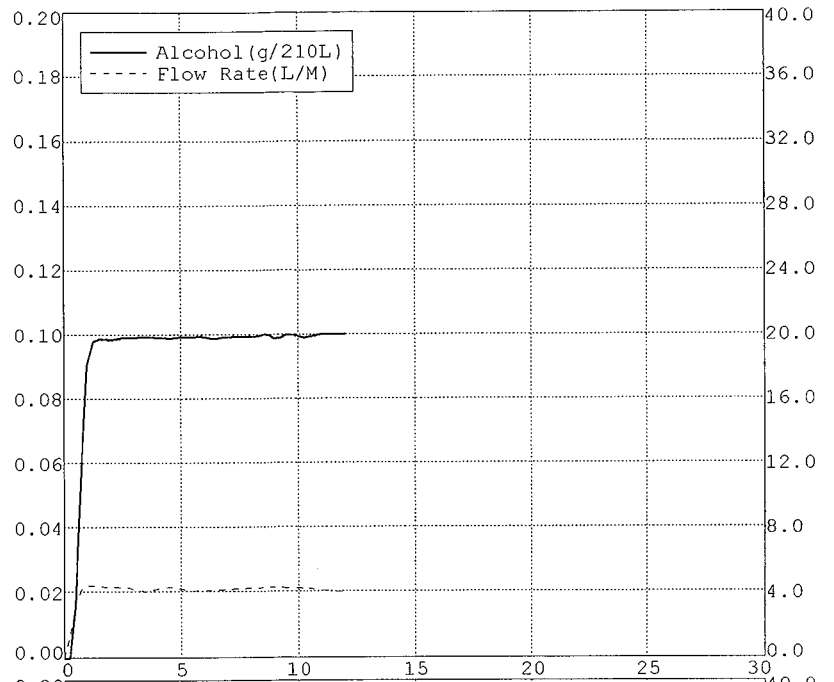

Hollie B Kennedy Rome PD 06/02/19
Rome City PD 10845

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 06/07/2019

OPERATOR NAME:
HOLLIE B KENNEDY
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:04
INTERNAL STANDARD	VERIFIED	21:04
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:04
BLANK TEST	0.00	21:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:06
BLANK TEST	0.00	21:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	21:07
BLANK TEST	0.00	21:08

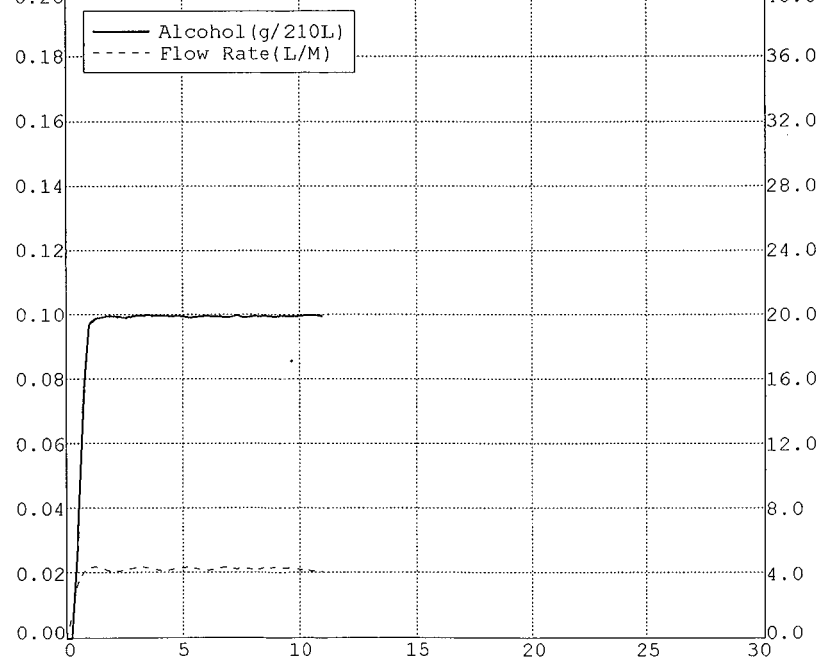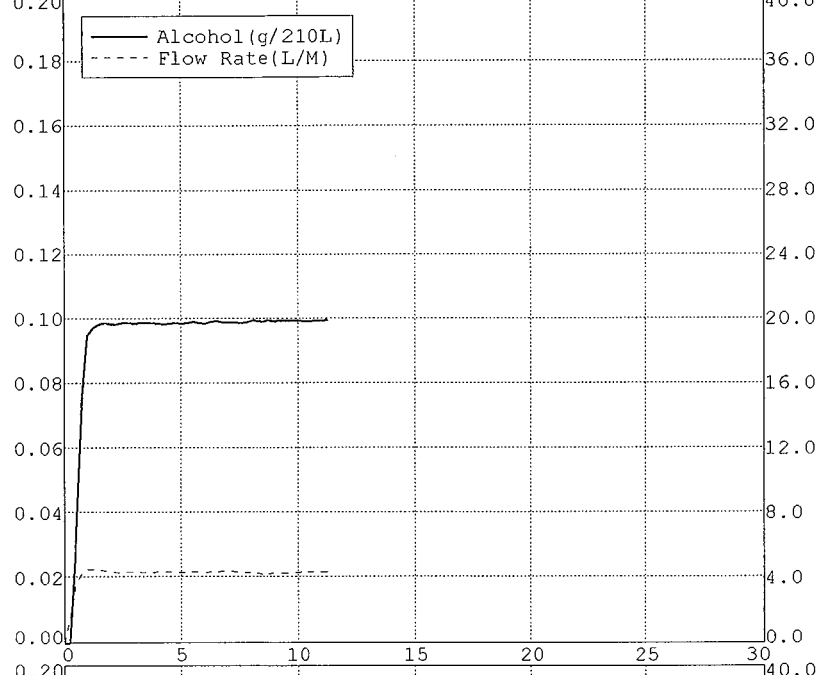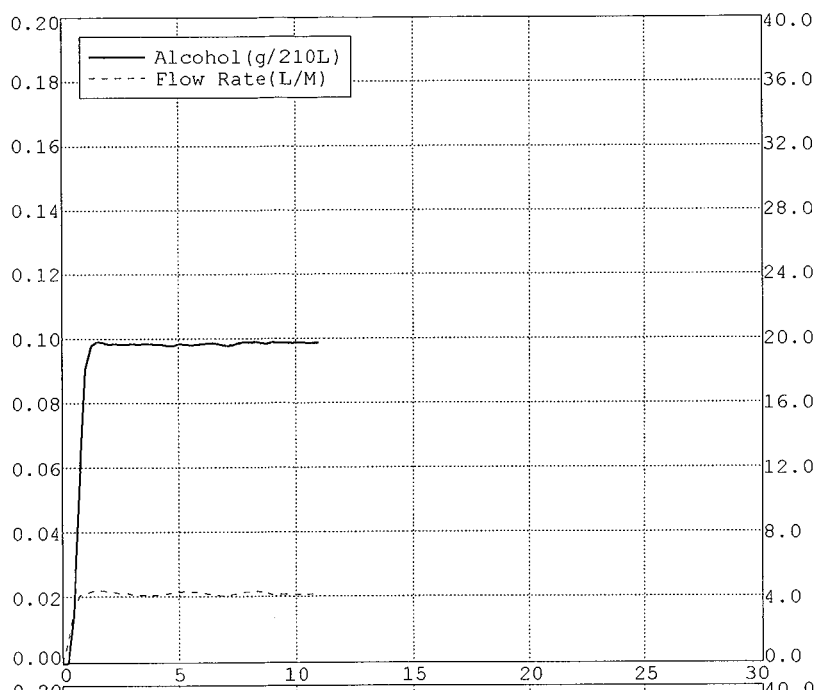

Hollie Kennedy Rome PD 2019
Rome Hollie Kennedy 10/19

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 06/14/2019

OPERATOR NAME:
HOLLIE B KENNEDY
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:14
INTERNAL STANDARD	VERIFIED	09:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:15
BLANK TEST	0.00	09:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:16
BLANK TEST	0.00	09:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:17
BLANK TEST	0.00	09:18

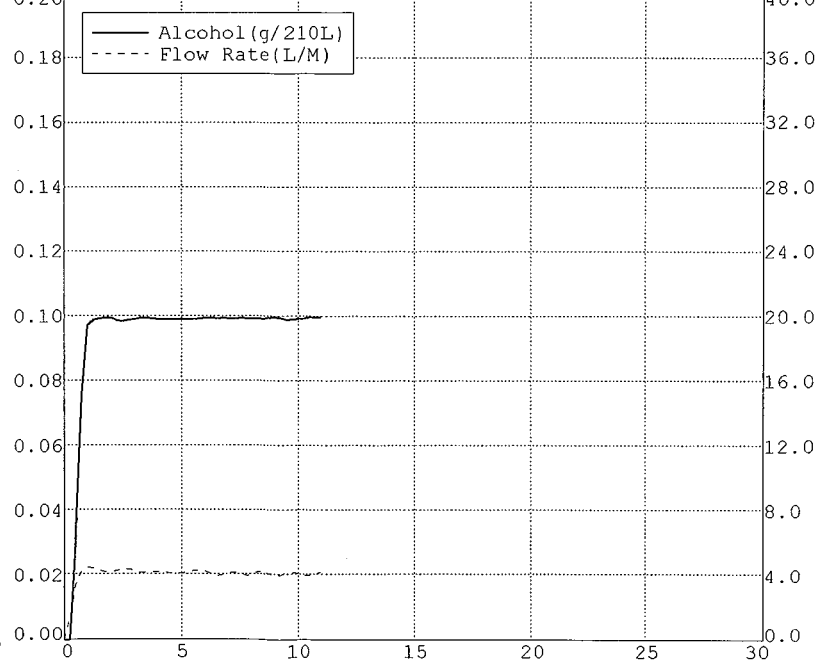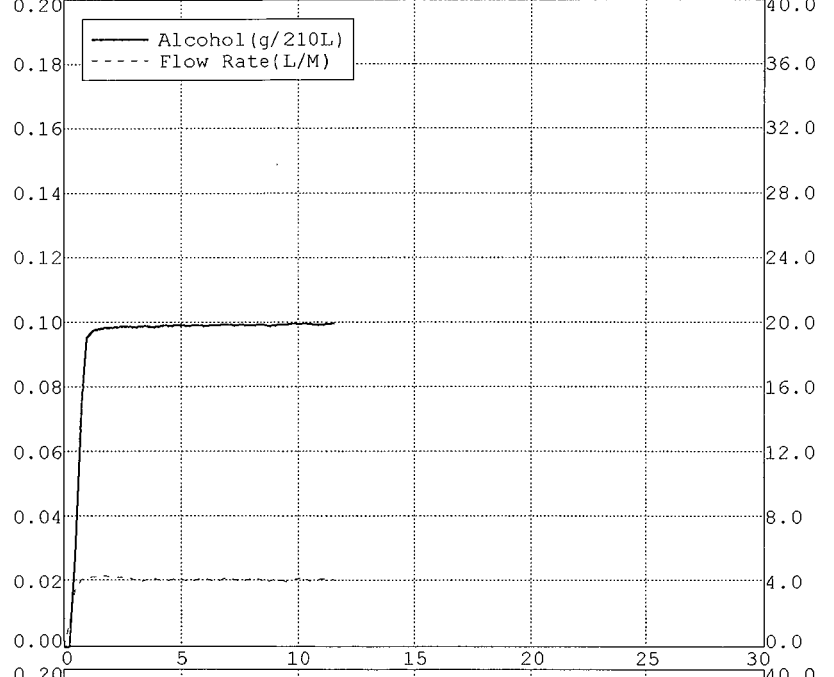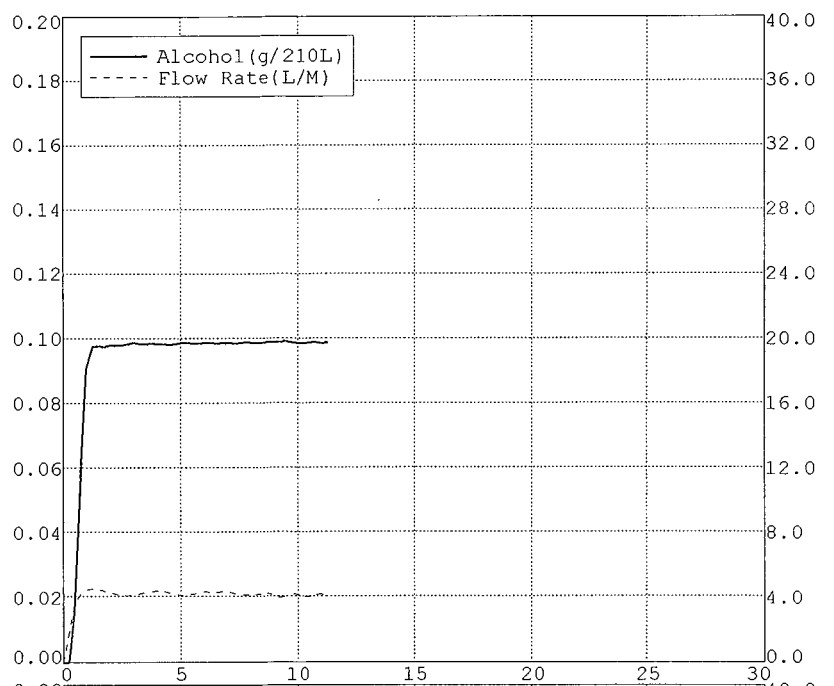

Hollie B Kennedy Rome PD 06/14/19
Hollie B Kennedy 10/15

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 06/22/2019

OPERATOR NAME:
HOLLIE B KENNEDY
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:01
INTERNAL STANDARD	VERIFIED	16:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:02
BLANK TEST	0.00	16:03
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:03
BLANK TEST	0.00	16:04
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:04
BLANK TEST	0.00	16:05

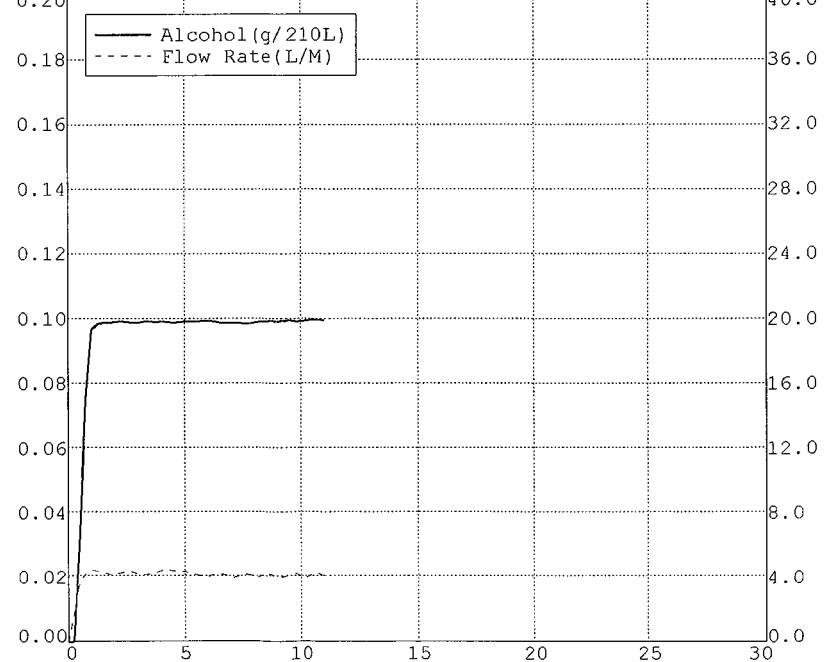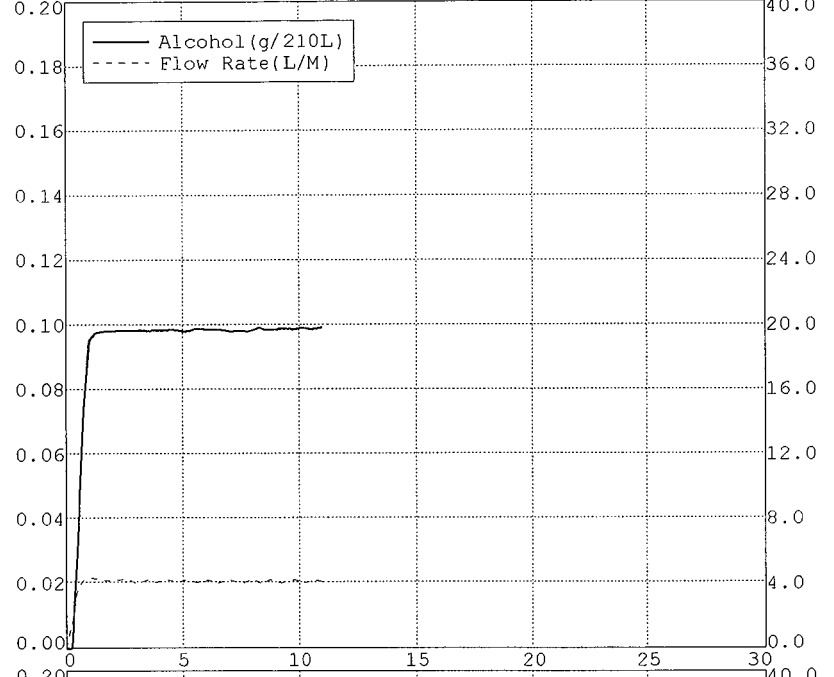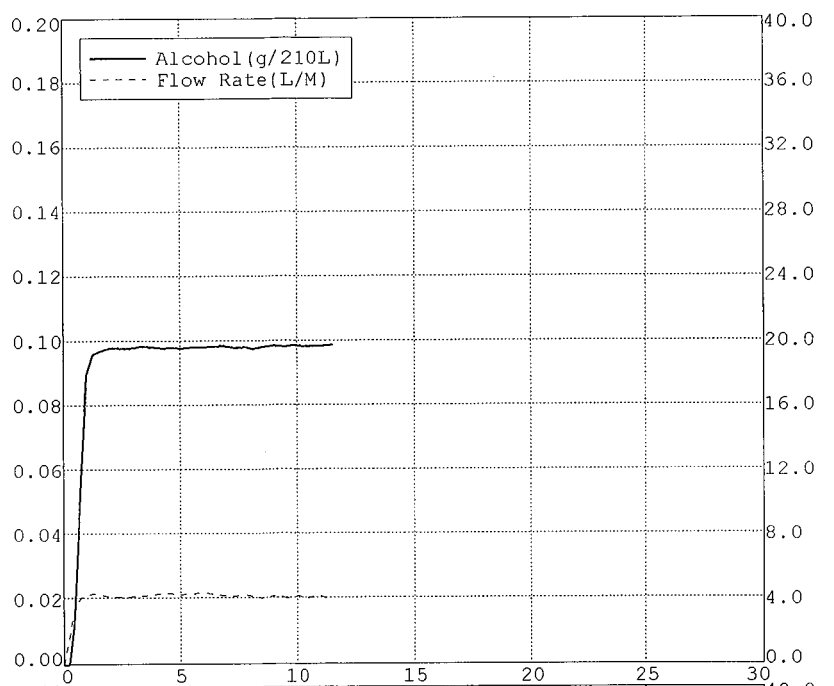

Hollie B Kennedy Rome PD 06/22/19
Hollie B Kennedy 10/25

SUPERVISOR TEST



ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 06/28/2019

OPERATOR NAME:
HOLLIE B KENNEDY
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:44
INTERNAL STANDARD	VERIFIED	16:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:44
BLANK TEST	0.00	16:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:45
BLANK TEST	0.00	16:46
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:46
BLANK TEST	0.00	16:47

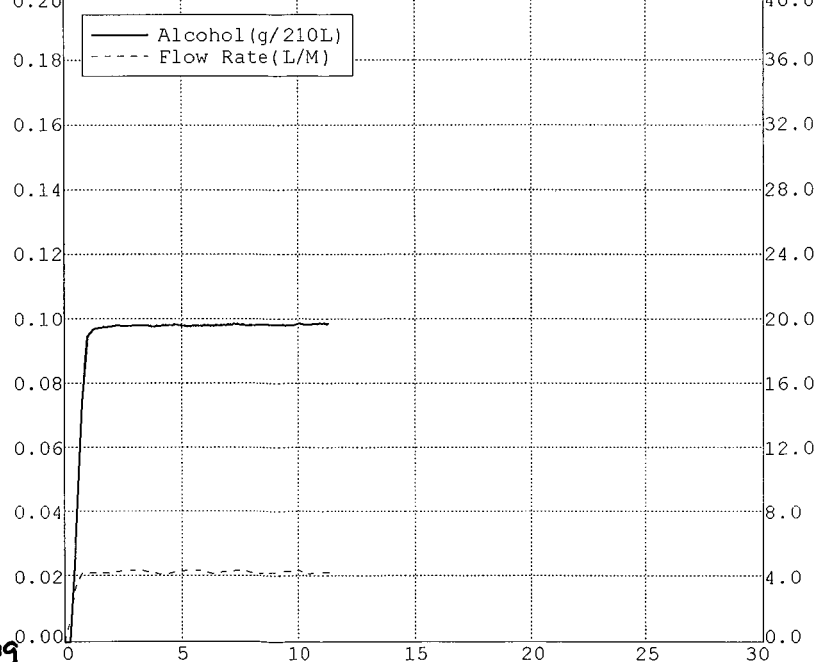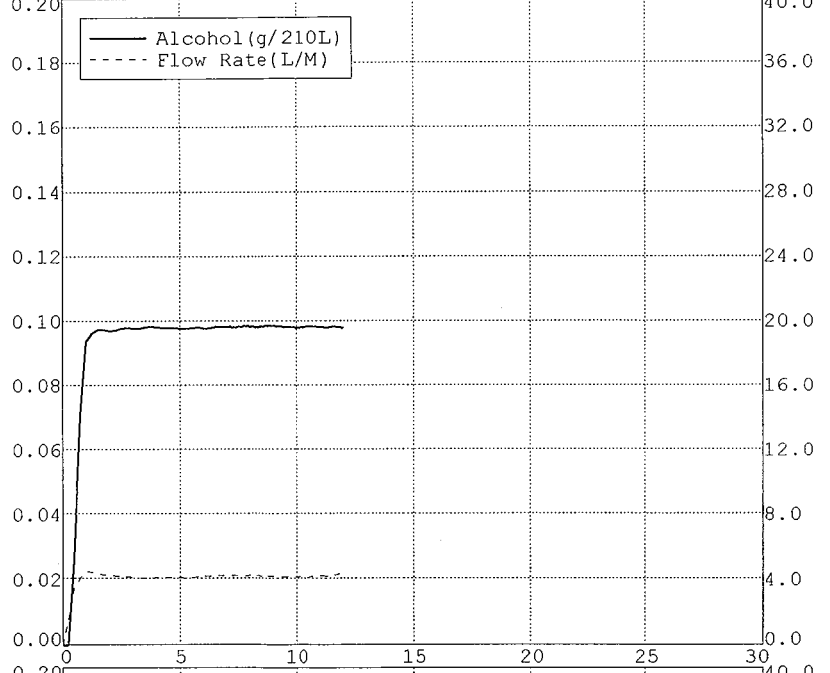

Hollie B. Silverman Rome PD 06/28/19
Hollie Silverman 10905