

SUPERVISOR TEST




ROME CITY
 POLICE DEPT
 DATAMASTER dmt: 106106

Date: 03/06/2020

OPERATOR NAME:
 HOLLIE B SILVERMAN
 Permit #: 39044
 Operator Agency/Dept: ROME CITY PD
 Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:33
INTERNAL STANDARD	VERIFIED	09:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:33
BLANK TEST	0.00	09:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:35
BLANK TEST	0.00	09:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:36
BLANK TEST	0.00	09:37

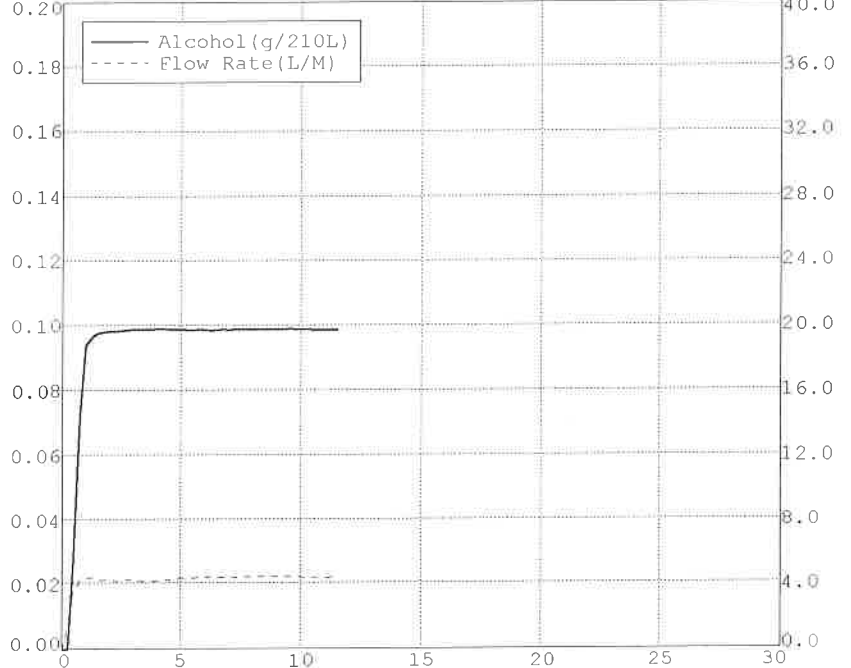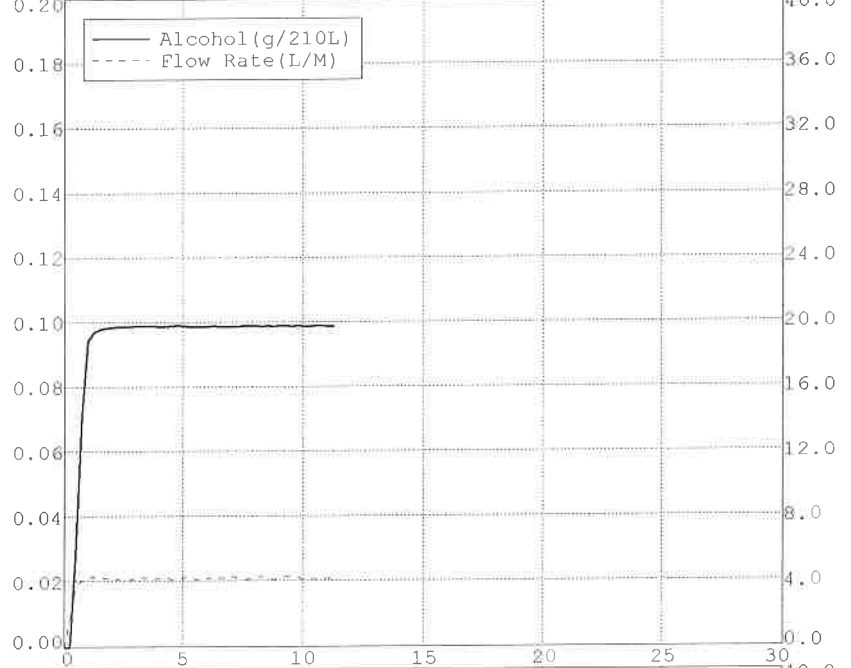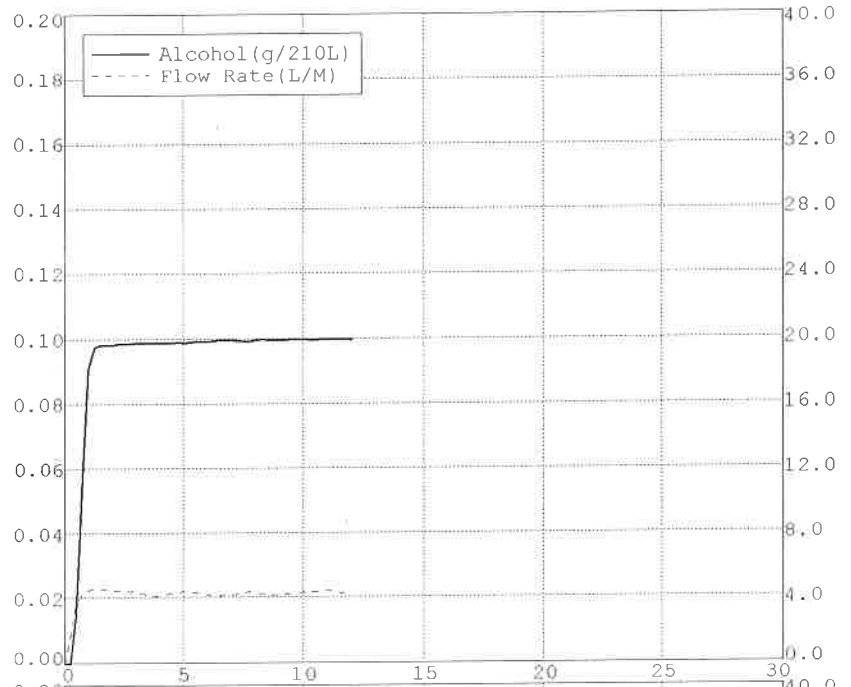

Hollie B. Silverman Rome PD 03/06/2020

~~Hollie B. Silverman~~ 10/21/20