

SUPERVISOR TEST



ROME CITY  
POLICE DEPT  
DATAMASTER dmt: 106106

Date: 03/13/2020

OPERATOR NAME:  
HOLLIE B SILVERMAN  
Permit #: 39044  
Operator Agency/Dept: ROME CITY PD  
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:56
INTERNAL STANDARD	VERIFIED	09:56
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:57
BLANK TEST	0.00	09:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:58
BLANK TEST	0.00	09:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:59
BLANK TEST	0.00	10:00

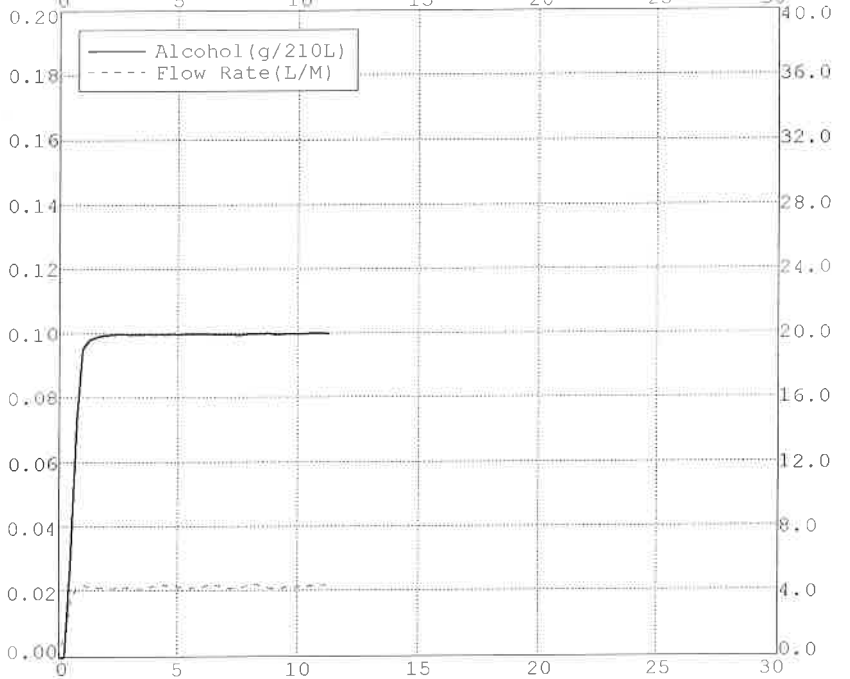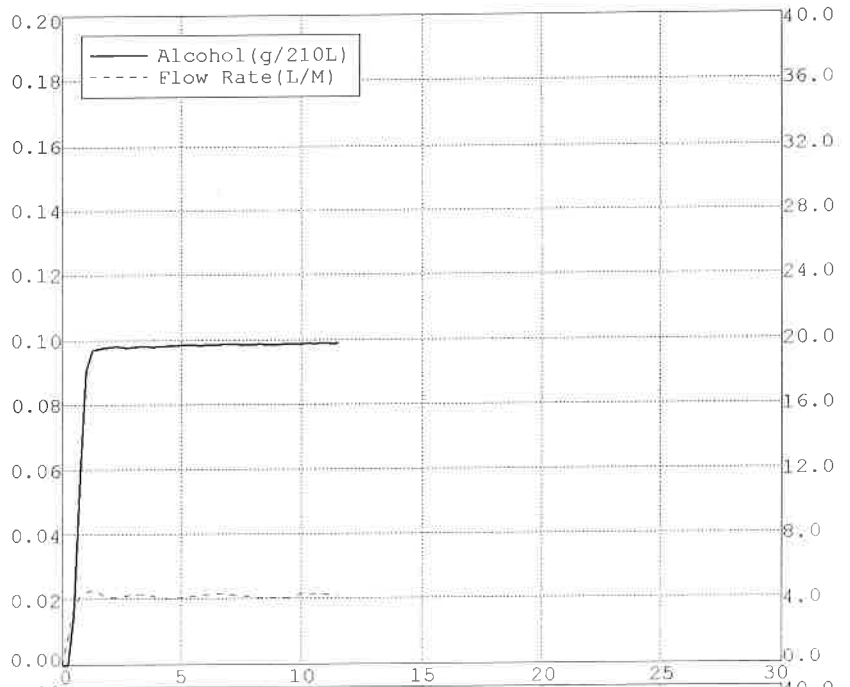

Hollie B. Silverman Rome PD 03/13/2020

Hollie B. Silverman 106106