

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 05/09/2020

OPERATOR NAME:
HOLLIE B SILVERMAN
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:27
INTERNAL STANDARD	VERIFIED	11:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:27
BLANK TEST	0.00	11:28
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:28
BLANK TEST	0.00	11:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:30
BLANK TEST	0.00	11:31

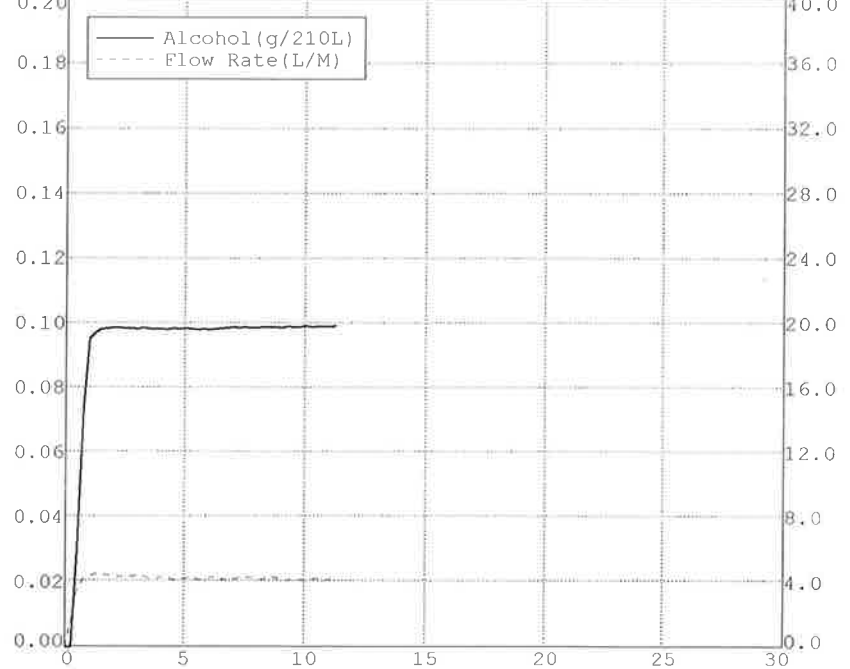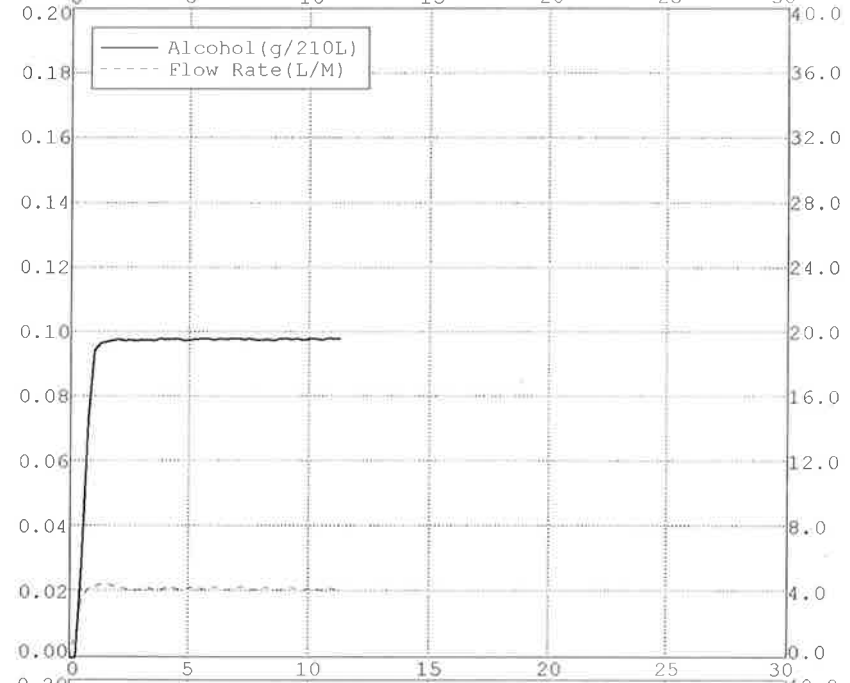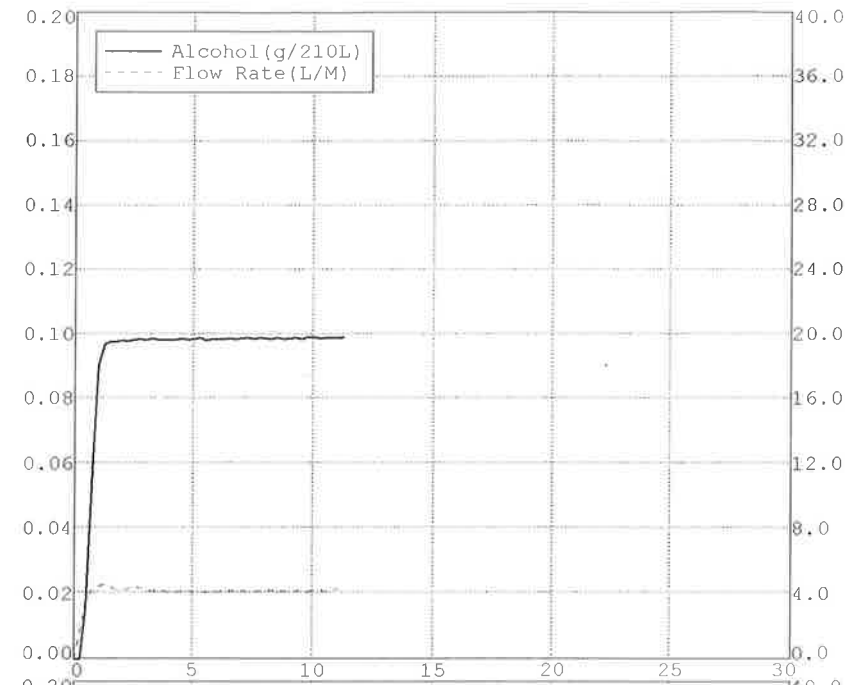

Hollie B. Silverman Rome PD 05/09/2020
Hollie B. Silverman 10/05