

SUPERVISOR TEST




SHERRILL CITY
POLICE DEPT
DATAMASTER dmt: 115108

Date: 11/06/2019

OPERATOR NAME:
ROBERT J DRAKE
Permit #: 27298
Operator Agency/Dept: SHERRILL CITY PD
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:50
INTERNAL STANDARD	VERIFIED	08:50
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:51
BLANK TEST	0.00	08:51
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:52
BLANK TEST	0.00	08:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:53
BLANK TEST	0.00	08:54



SOLUTION CHANGE




SHERRILL CITY
POLICE DEPT
DATAMASTER dmt: 115108

ate: 10/30/2019

OPERATOR NAME:
ROBERT J DRAKE
Permit #: 27298
Operator Agency/Dept: SHERRILL CITY PD
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:50
INTERNAL STANDARD	VERIFIED	07:50
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:51
BLANK TEST	0.00	07:52
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:52
BLANK TEST	0.00	07:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:53
BLANK TEST	0.00	07:54



SUPERVISOR TEST




SHERRILL CITY
POLICE DEPT
DATAMASTER dmt: 115108

Date: 10/23/2019

OPERATOR NAME:
JOSEPH A PRUCKNO
Permit #: 43761
Operator Agency/Dept: SHERRILL CITY PD
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:35
INTERNAL STANDARD	VERIFIED	04:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	04:35
BLANK TEST	0.00	04:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	04:36
BLANK TEST	0.00	04:37
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	04:38
BLANK TEST	0.00	04:39



SUPERVISOR TEST




SHERRILL CITY
POLICE DEPT
DATAMASTER dmt: 115108

Date: 10/16/2019

OPERATOR NAME:
JOSEPH A PRUCKNO
Permit #: 43761
Operator Agency/Dept: SHERRILL CITY PD
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:54
INTERNAL STANDARD	VERIFIED	04:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	04:55
BLANK TEST	0.00	04:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	04:56
BLANK TEST	0.00	04:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	04:57
BLANK TEST	0.00	04:58



SUPERVISOR TEST




SHERRILL CITY
POLICE DEPT
DATAMASTER dmt: 115108

Date: 10/09/2019

OPERATOR NAME:
ROBERT J DRAKE
Permit #: 27298
Operator Agency/Dept: SHERRILL CITY PD
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:58
INTERNAL STANDARD	VERIFIED	06:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	06:59
BLANK TEST	0.00	07:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:00
BLANK TEST	0.00	07:01
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:01
BLANK TEST	0.00	07:02



SOLUTION CHANGE




SHERRILL CITY
POLICE DEPT
DATAMASTER dmt: 115108

Date: 10/01/2019

OPERATOR NAME:
ROBERT J DRAKE
Permit #: 27298
Operator Agency/Dept: SHERRILL CITY PD
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:55
INTERNAL STANDARD	VERIFIED	07:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:56
BLANK TEST	0.00	07:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:57
BLANK TEST	0.00	07:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:58
BLANK TEST	0.00	07:59



SUPERVISOR TEST




SHERRILL CITY
POLICE DEPT
DATAMASTER dmt: 115108

Date: 09/25/2019

OPERATOR NAME:
ROBERT J DRAKE
Permit #: 27298
Operator Agency/Dept: SHERRILL CITY PD
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:48
INTERNAL STANDARD	VERIFIED	06:48
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	06:48
BLANK TEST	0.00	06:49
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	06:50
BLANK TEST	0.00	06:50
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	06:51
BLANK TEST	0.00	06:52



SUPERVISOR TEST




SHERRILL CITY
POLICE DEPT
DATAMASTER dmt: 115108

ate: 09/18/2019

OPERATOR NAME:
ROBERT J DRAKE
Permit #: 27298
Operator Agency/Dept: SHERRILL CITY PD
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:20
INTERNAL STANDARD	VERIFIED	07:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:21
BLANK TEST	0.00	07:22
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:22
BLANK TEST	0.00	07:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:23
BLANK TEST	0.00	07:24



SUPERVISOR TEST




 SHERRILL CITY
 POLICE DEPT
 DATAMASTER dmt: 115108

Date: 09/11/2019

OPERATOR NAME:
 JOSEPH A PRUCKNO
 Permit #: 43761
 Operator Agency/Dept: SHERRILL CITY PD
 Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:50
INTERNAL STANDARD	VERIFIED	06:50
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:50
BLANK TEST	0.00	06:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:51
BLANK TEST	0.00	06:52
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:52
BLANK TEST	0.00	06:53



SOLUTION CHANGE




SHERRILL CITY
POLICE DEPT
DATAMASTER dmt: 115108

Date: 09/03/2019

OPERATOR NAME:
ROBERT J DRAKE
Permit #: 27298
Operator Agency/Dept: SHERRILL CITY PD
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:34
INTERNAL STANDARD	VERIFIED	07:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:34
BLANK TEST	0.00	07:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:36
BLANK TEST	0.00	07:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:37
BLANK TEST	0.00	07:38



SUPERVISOR TEST




SHERRILL CITY
POLICE DEPT
DATAMASTER dmt: 115108

Date: 08/28/2019

OPERATOR NAME:
ROBERT J DRAKE
Permit #: 27298
Operator Agency/Dept: SHERRILL CITY PD
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:10
INTERNAL STANDARD	VERIFIED	07:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:11
BLANK TEST	0.00	07:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:12
BLANK TEST	0.00	07:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:13
BLANK TEST	0.00	07:14



SUPERVISOR TEST




SHERRILL CITY
POLICE DEPT
DATAMASTER dmt: 115108

Date: 08/21/2019

OPERATOR NAME:
ROBERT J DRAKE
Permit #: 27298
Operator Agency/Dept: SHERRILL CITY PD
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:23
INTERNAL STANDARD	VERIFIED	07:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:24
BLANK TEST	0.00	07:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:25
BLANK TEST	0.00	07:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:26
BLANK TEST	0.00	07:27



SUPERVISOR TEST




SHERRILL CITY
POLICE DEPT
DATAMASTER dmt: 115108

Date: 08/14/2019

OPERATOR NAME:
SHAWN R PLATT
Permit #: 30289
Operator Agency/Dept: SHERRILL CITY PD
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:00
INTERNAL STANDARD	VERIFIED	07:01
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:01
BLANK TEST	0.00	07:02
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:02
BLANK TEST	0.00	07:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:03
BLANK TEST	0.00	07:04



SUPERVISOR TEST




SHERRILL CITY
POLICE DEPT
DATAMASTER dmt: 115108

Date: 08/07/2019

OPERATOR NAME:
ROBERT J DRAKE
Permit #: 27298
Operator Agency/Dept: SHERRILL CITY PD
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:18
INTERNAL STANDARD	VERIFIED	09:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:19
BLANK TEST	0.00	09:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:20
BLANK TEST	0.00	09:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:21
BLANK TEST	0.00	09:22



SOLUTION CHANGE




SHERRILL CITY
POLICE DEPT
DATAMASTER dmt: 115108

Date: 08/01/2019

OPERATOR NAME:
ROBERT J DRAKE
Permit #: 27298
Operator Agency/Dept: SHERRILL CITY PD
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:55
INTERNAL STANDARD	VERIFIED	07:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:55
BLANK TEST	0.00	07:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:56
BLANK TEST	0.00	07:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:58
BLANK TEST	0.00	07:58



SUPERVISOR TEST




SHERRILL CITY
POLICE DEPT
DATAMASTER dmt: 115108

ate: 07/31/2019

OPERATOR NAME:
JOSEPH A PRUCKNO
Permit #: 43761
Operator Agency/Dept: SHERRILL CITY PD
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:23
INTERNAL STANDARD	VERIFIED	03:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	03:23
BLANK TEST	0.00	03:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:25
BLANK TEST	0.00	03:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:26
BLANK TEST	0.00	03:27



SUPERVISOR TEST




SHERRILL CITY
POLICE DEPT
DATAMASTER dmt: 115108

Date: 07/24/2019

OPERATOR NAME:
JOSEPH A PRUCKNO
Permit #: 43761
Operator Agency/Dept: SHERRILL CITY PD
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:43
INTERNAL STANDARD	VERIFIED	06:43
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:43
BLANK TEST	0.00	06:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	06:44
BLANK TEST	0.00	06:45
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:45
BLANK TEST	0.00	06:46



SUPERVISOR TEST




SHERRILL CITY
POLICE DEPT
DATAMASTER dmt: 115108

Date: 07/17/2019

OPERATOR NAME:
JOSEPH A PRUCKNO
Permit #: 43761
Operator Agency/Dept: SHERRILL CITY PD
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:49
INTERNAL STANDARD	VERIFIED	06:49
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	06:49
BLANK TEST	0.00	06:50
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	06:50
BLANK TEST	0.00	06:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:52
BLANK TEST	0.00	06:53



SUPERVISOR TEST




SHERRILL CITY
POLICE DEPT
DATAMASTER dmt: 115108

Date: 07/10/2019

OPERATOR NAME:
JOSEPH A PRUCKNO
Permit #: 43761
Operator Agency/Dept: SHERRILL CITY PD
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:31
INTERNAL STANDARD	VERIFIED	06:31
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:32
BLANK TEST	0.00	06:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:33
BLANK TEST	0.00	06:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:34
BLANK TEST	0.00	06:35

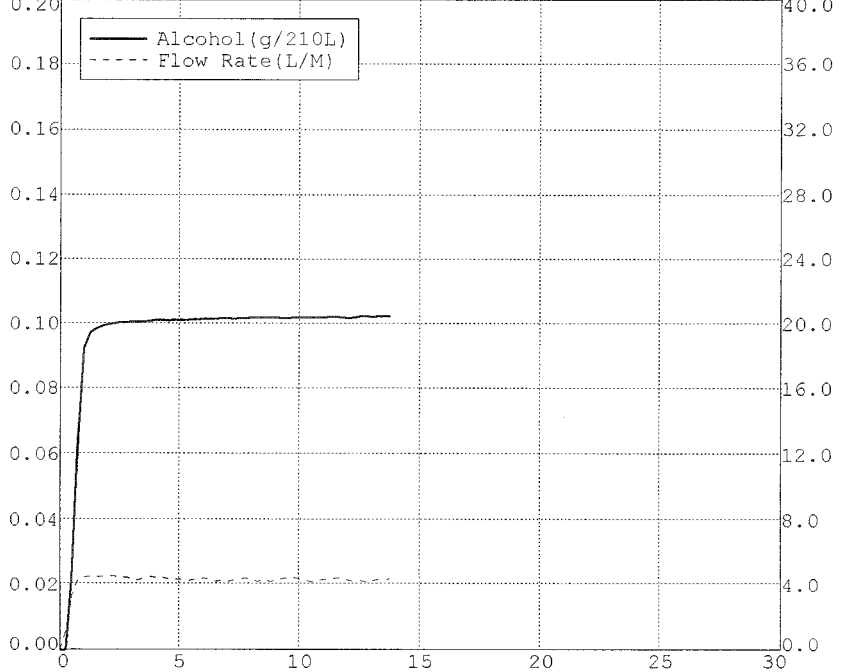

SUPERVISOR TEST




SHERRILL CITY
POLICE DEPT
DATAMASTER dmt: 115108

Date: 07/03/2019

OPERATOR NAME:
JOSEPH A PRUCKNO
Permit #: 43761
Operator Agency/Dept: SHERRILL CITY PD
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:11
INTERNAL STANDARD	VERIFIED	08:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:11
BLANK TEST	0.00	08:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:13
BLANK TEST	0.00	08:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:14
BLANK TEST	0.00	08:15



SUPERVISOR TEST

SHERRILL CITY
POLICE DEPT
DATAMASTER dmt: 115108

Date: 07/01/2019

OPERATOR NAME:
ROBERT J DRAKE
Permit #: 27298
Operator Agency/Dept: SHERRILL CITY PD
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:41
INTERNAL STANDARD	VERIFIED	09:41
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:41
BLANK TEST	0.00	09:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:42
BLANK TEST	0.00	09:43
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:44
BLANK TEST	0.00	09:45

