

SUPERVISOR TEST

UTICA CITY  
POLICE DEPT  
DATAMASTER dmt: 107308




Date: 01/07/2020

*RMS*  
*20-660*

OPERATOR NAME:  
MICHAEL J CLIVE  
Permit #: 36682  
Operator Agency/Dept: UTICA CITY PD  
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:56
INTERNAL STANDARD	VERIFIED	11:56
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	11:56
BLANK TEST	0.00	11:57
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	11:57
BLANK TEST	0.00	11:58
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	11:58
BLANK TEST	0.00	11:59

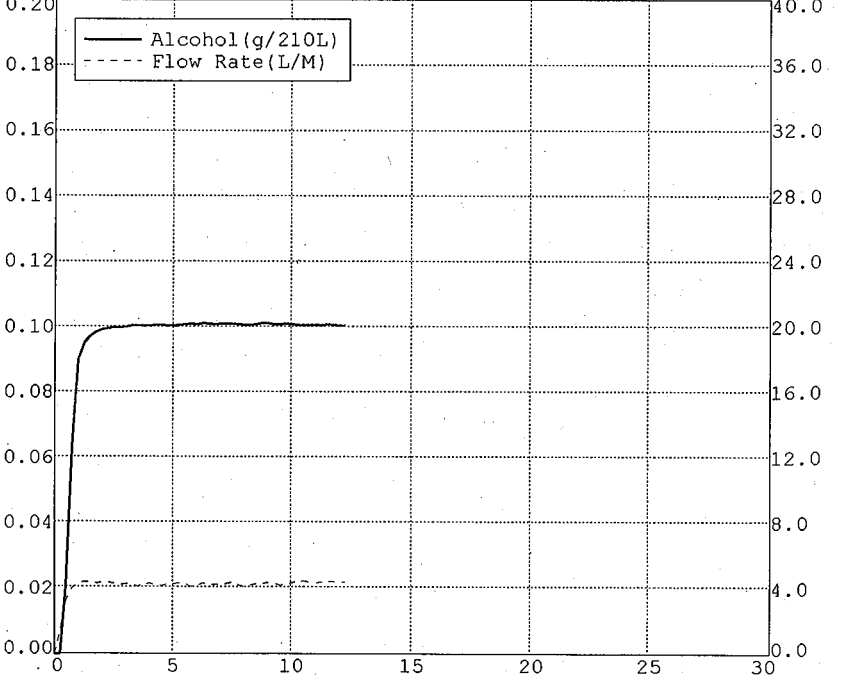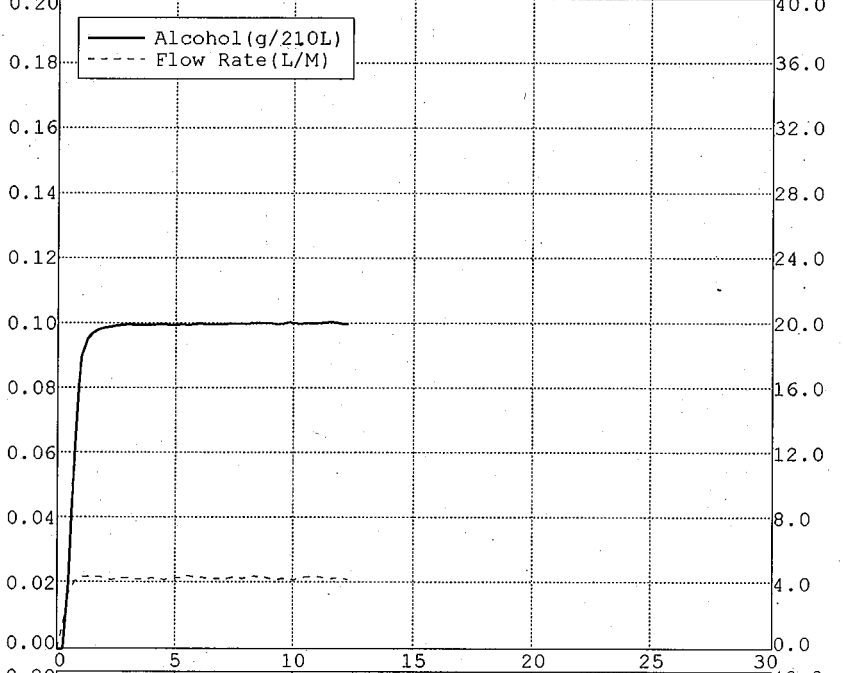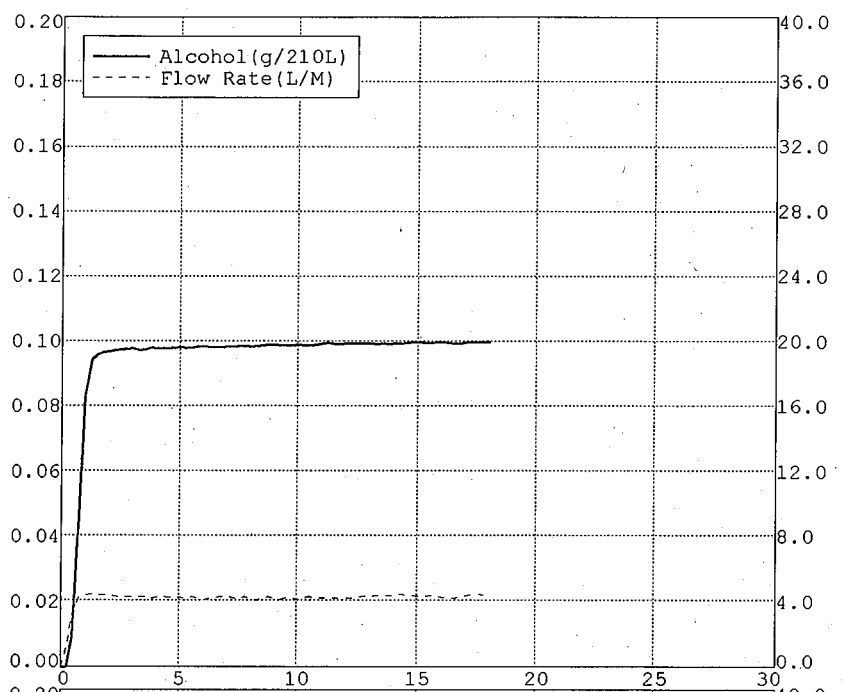

SUPERVISOR TEST

UTICA CITY  
POLICE DEPT  
DATAMASTER dmt: 100282

Date: 01/07/2020

*RM*  
*20-660*

OPERATOR NAME:  
MICHAEL J CLIVE  
Permit #: 366682  
Operator Agency/Dept: UTICA CITY PD  
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:41
INTERNAL STANDARD	VERIFIED	11:41
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	11:42
BLANK TEST	0.00	11:42
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	11:43
BLANK TEST	0.00	11:43
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:44
BLANK TEST	0.00	11:45

