

SUPERVISOR TEST

UTICA CITY
 POLICE DEPT
 DATAMASTER dmt: 100282




Date: 04/14/2020

RM's
 20-12236

OPERATOR NAME:
 MICHAEL J CLIVE
 Permit #: 36682
 Operator Agency/Dept: UTICA CITY PD
 Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:33
INTERNAL STANDARD	VERIFIED	12:33
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	12:33
BLANK TEST	0.00	12:34
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	12:34
BLANK TEST	0.00	12:35
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	12:35
BLANK TEST	0.00	12:36

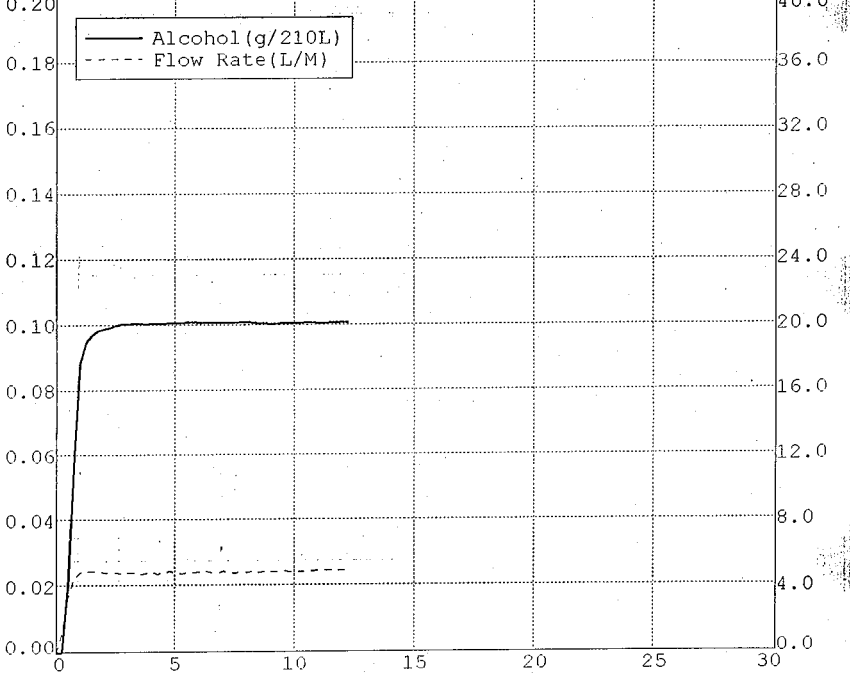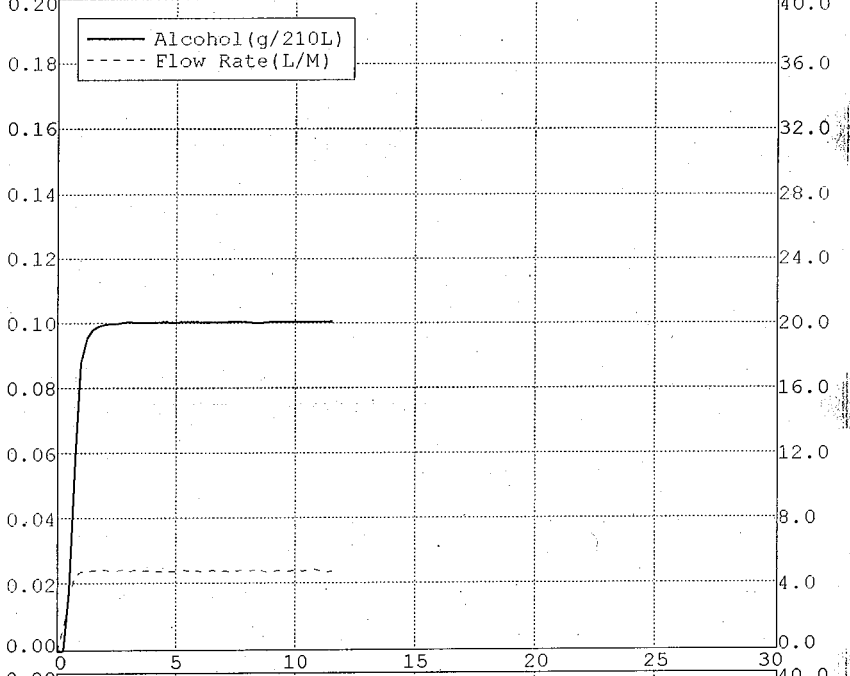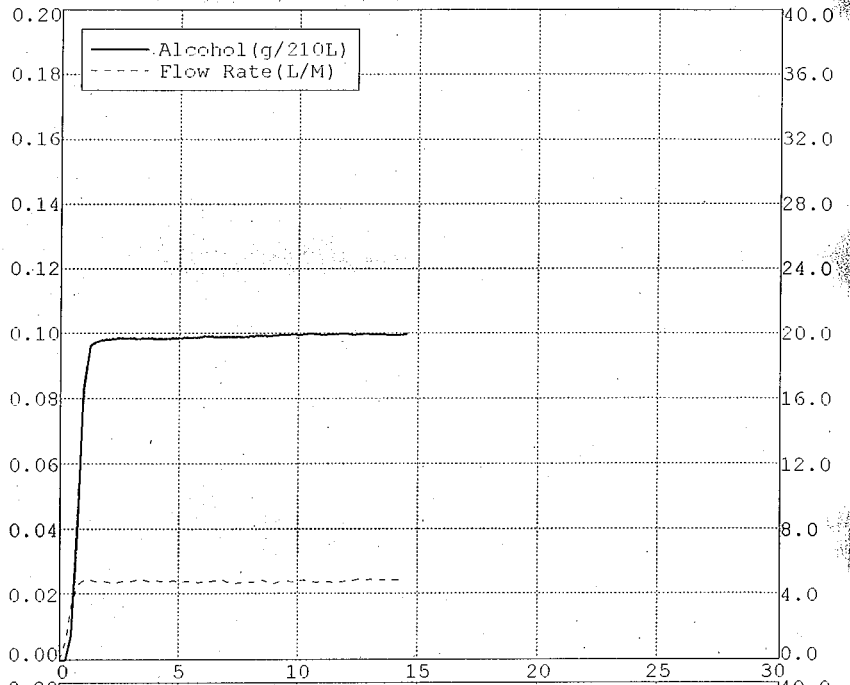

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308

Date: 04/14/2020

CM
20-12236

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:33
INTERNAL STANDARD	VERIFIED	12:33
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:34
BLANK TEST	0.00	12:35
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:35
BLANK TEST	0.00	12:36
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:36
BLANK TEST	0.00	12:37

