

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308




AMS
20-16490

Date: 05/19/2020

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:55
INTERNAL STANDARD	VERIFIED	11:55
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	11:56
BLANK TEST	0.00	11:56
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	11:57
BLANK TEST	0.00	11:58
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	11:58
BLANK TEST	0.00	11:59

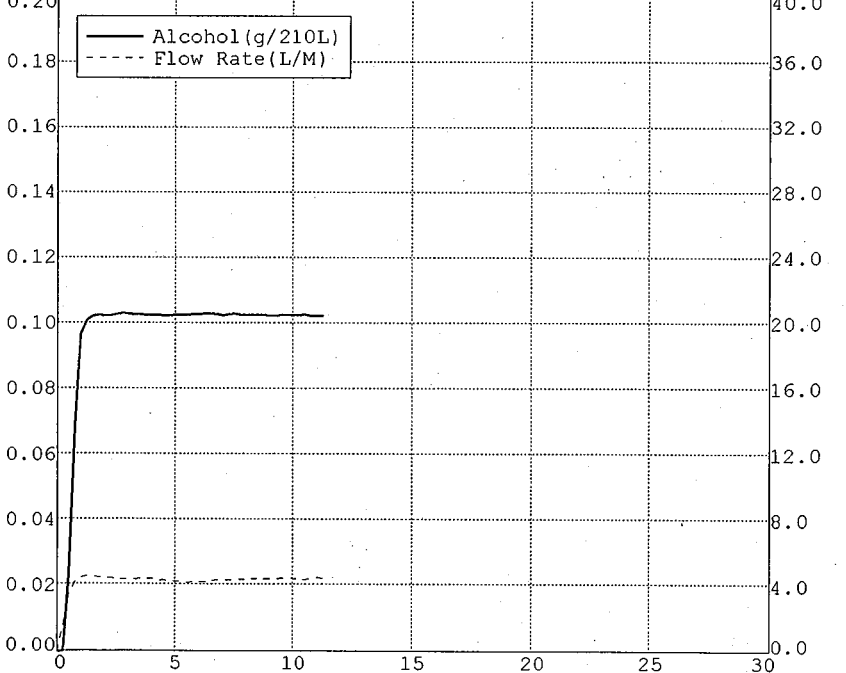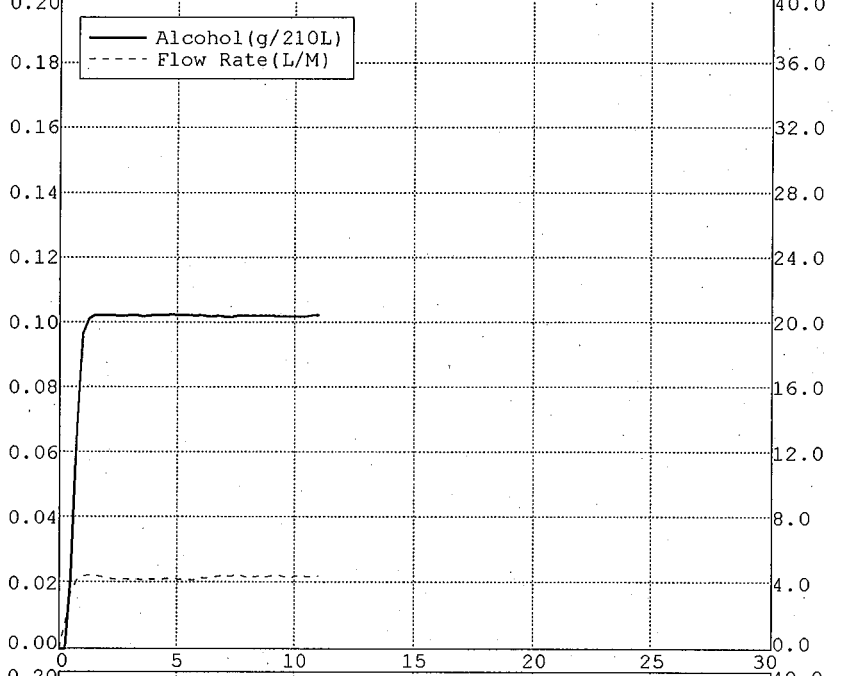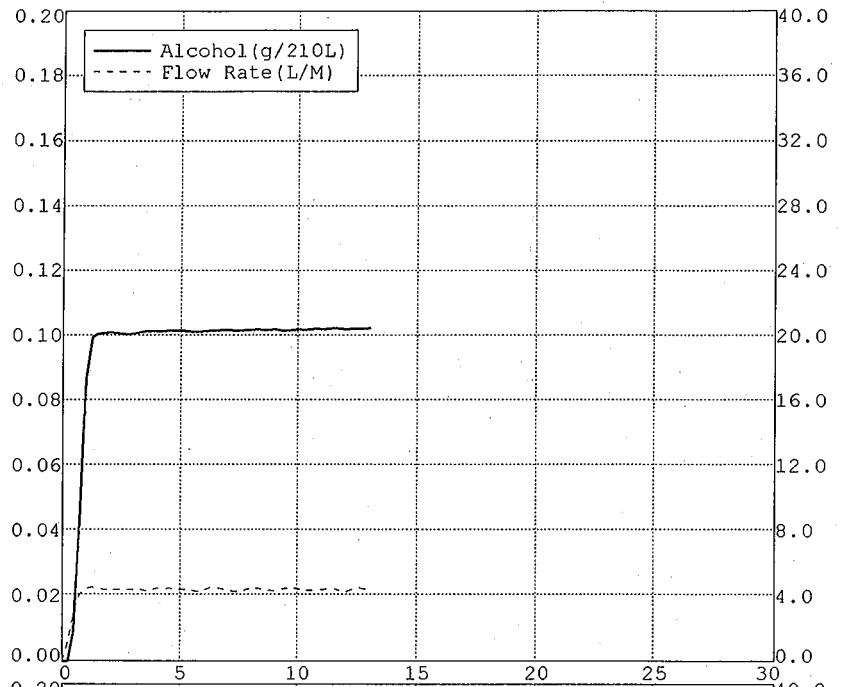

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282

Date: 05/19/2020

RMS
20-16490

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:49
INTERNAL STANDARD	VERIFIED	11:49
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	11:50
BLANK TEST	0.00	11:50
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	11:51
BLANK TEST	0.00	11:51
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	11:52
BLANK TEST	0.00	11:53

