

SUPERVISOR TEST




WHITESTOWN TOWN
POLICE DEPT.
DATAMASTER dmt: 100231

Date: 10/29/2019

OPERATOR NAME:
D J HUMPHRIES II
Permit #: 40440
Operator Agency/Dept: WHITESTOWN TOWN PD
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:28
INTERNAL STANDARD	VERIFIED	16:28
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	16:29
BLANK TEST	0.00	16:29
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	16:30
BLANK TEST	0.00	16:31
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	16:31
BLANK TEST	0.00	16:32

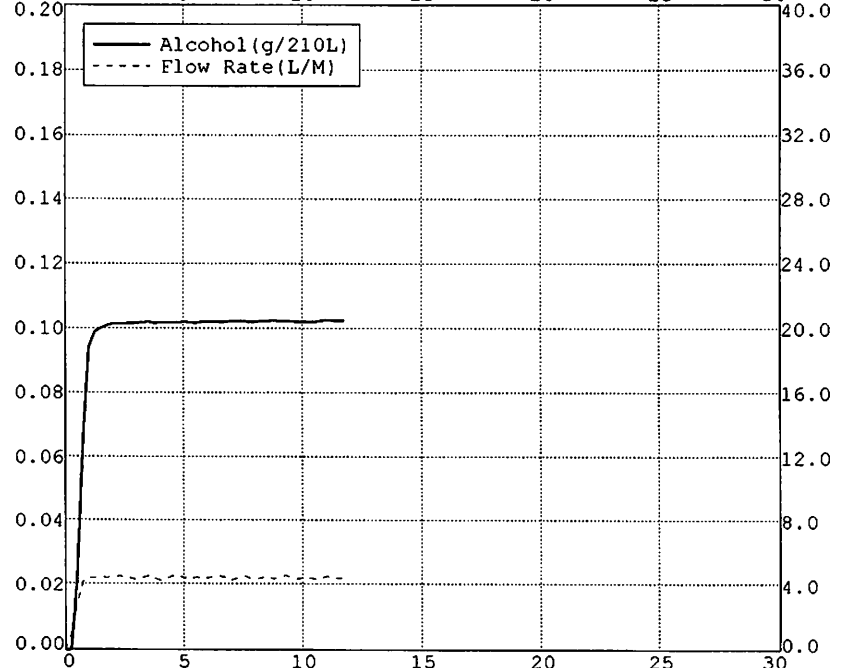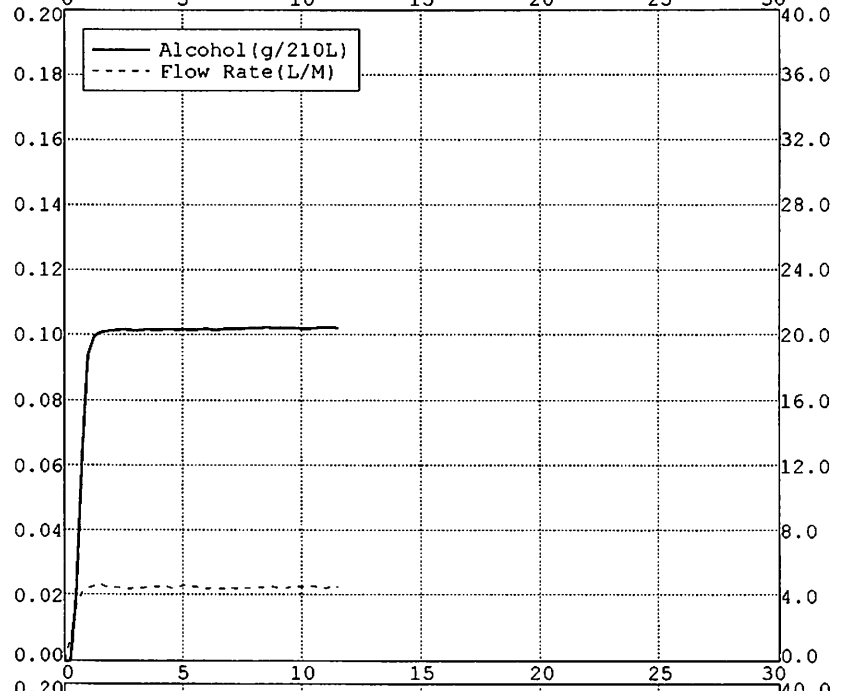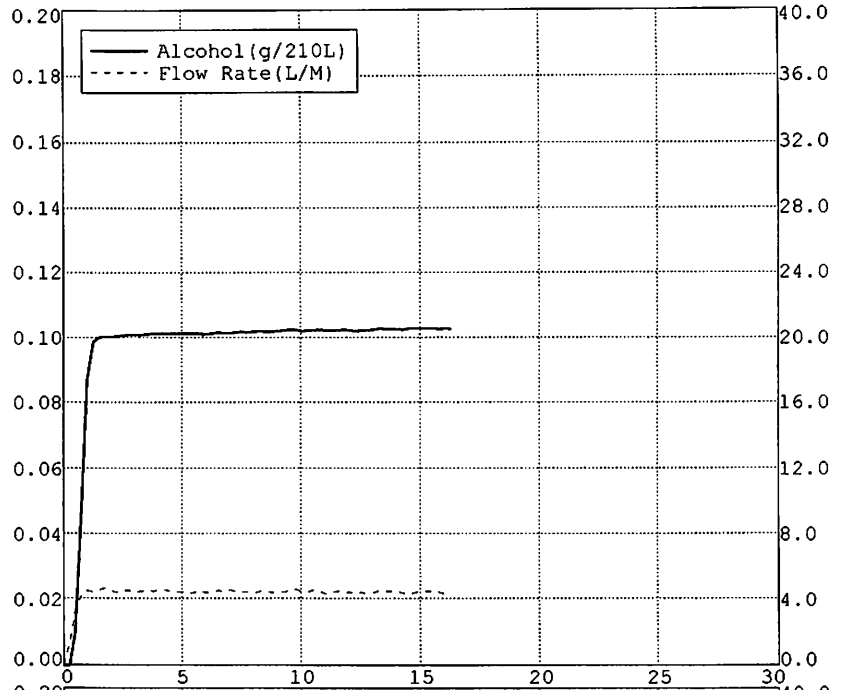

SUPERVISOR TEST




WHITESTOWN TOWN
POLICE DEPT.
DATAMASTER dmt: 100231

Date: 10/22/2019

OPERATOR NAME:
D J HUMPHRIES II
Permit #: 40440
Operator Agency/Dept: WHITESTOWN PD
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:02
INTERNAL STANDARD	VERIFIED	23:02
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	23:02
BLANK TEST	0.00	23:03
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	23:03
BLANK TEST	0.00	23:04
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	23:04
BLANK TEST	0.00	23:05

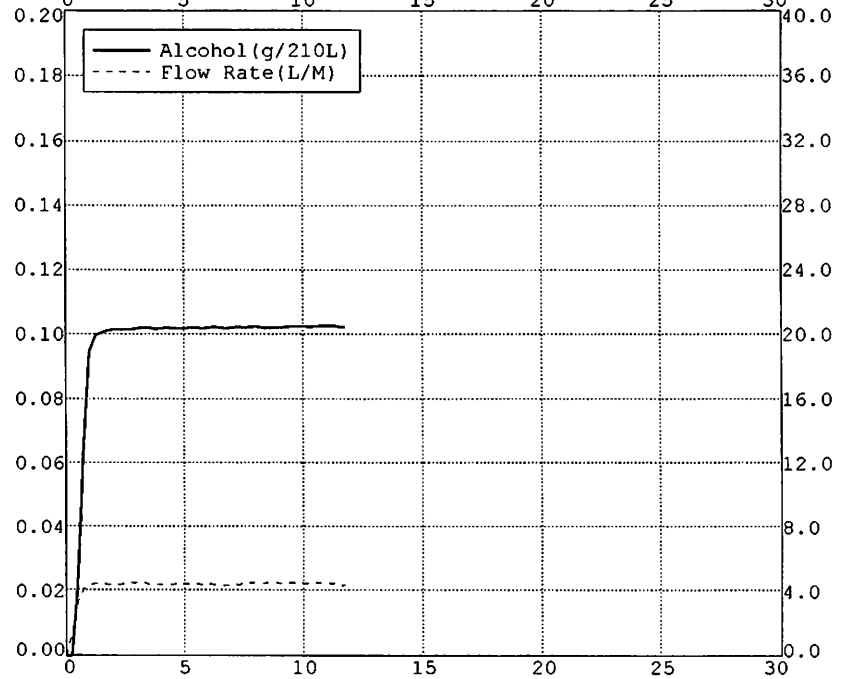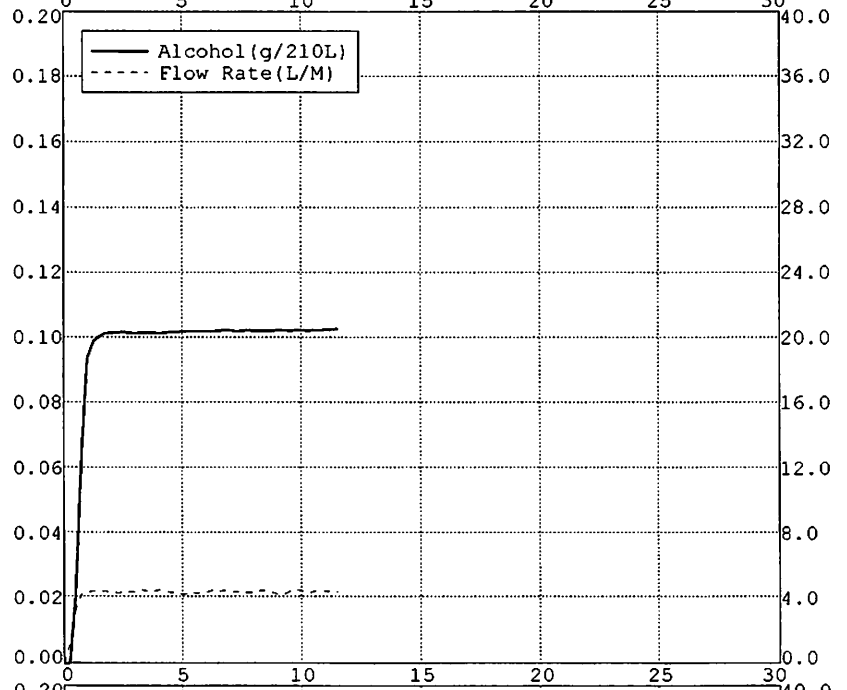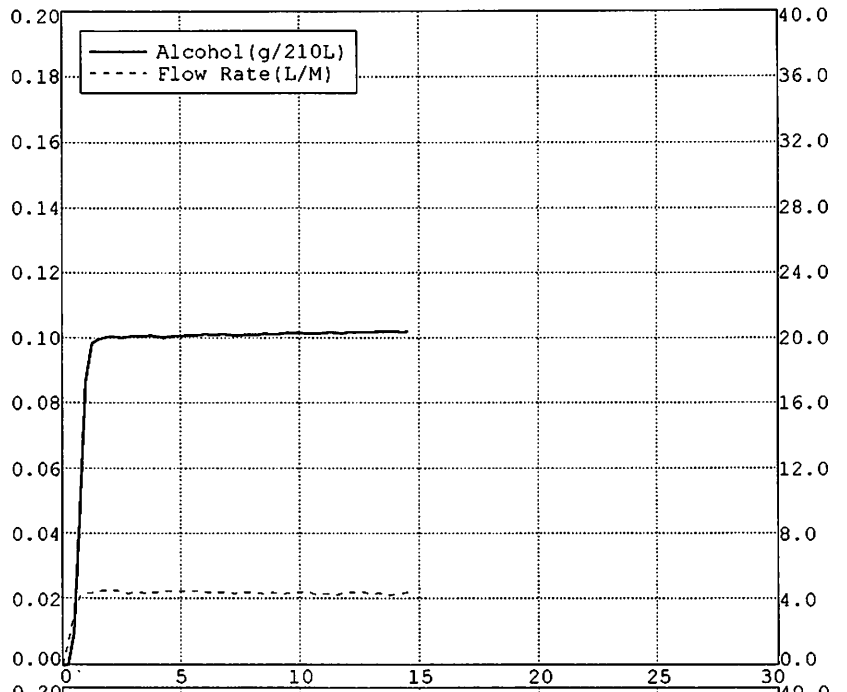

SOLUTION CHANGE

WHITESTOWN TOWN
POLICE DEPT.
DATAMASTER dmt: 100231

Date: 10/09/2019

OPERATOR NAME:
DAVID J HUMPHRIES II
Permit #: 40440
Operator Agency/Dept: WHITESTOWN TOWN PD
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:47
INTERNAL STANDARD	VERIFIED	14:47
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	14:47
BLANK TEST	0.00	14:48
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	14:49
BLANK TEST	0.00	14:49
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	14:50
BLANK TEST	0.00	14:51

SOLUTION CHANGE
AFTER REPAIRS

