

SUPERVISOR TEST

NEW HARTFORD TOWN

DATAMASTER dmt: 127606

Date: 07/08/2020

OPERATOR NAME:

MICHAEL T KOWALSKI




Permit #: 31077

Operator Agency/Dept: NEW HARTFORD TOWN PD

Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:14
INTERNAL STANDARD	VERIFIED	14:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:14
BLANK TEST	0.00	14:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:16
BLANK TEST	0.00	14:16
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	14:17
BLANK TEST	0.00	14:18

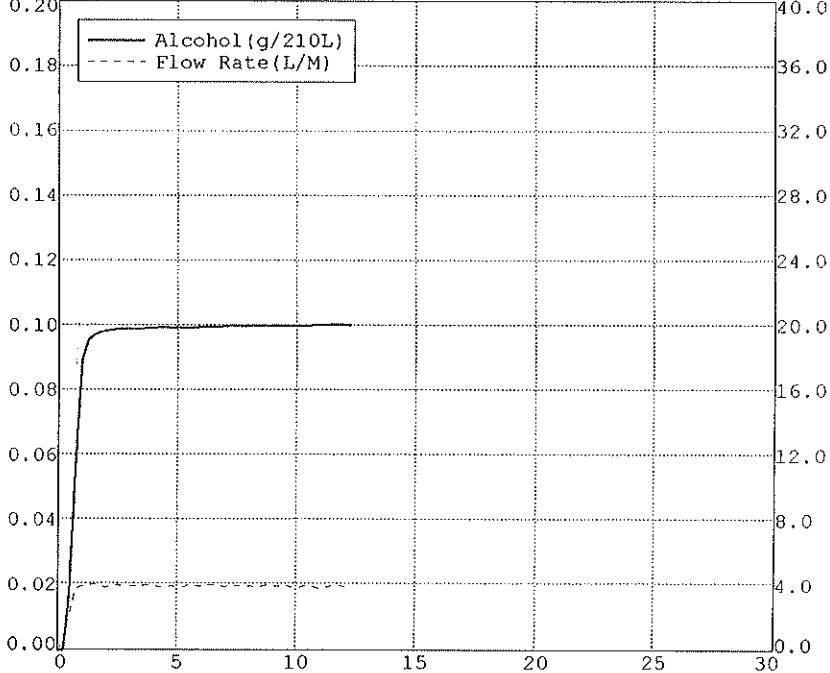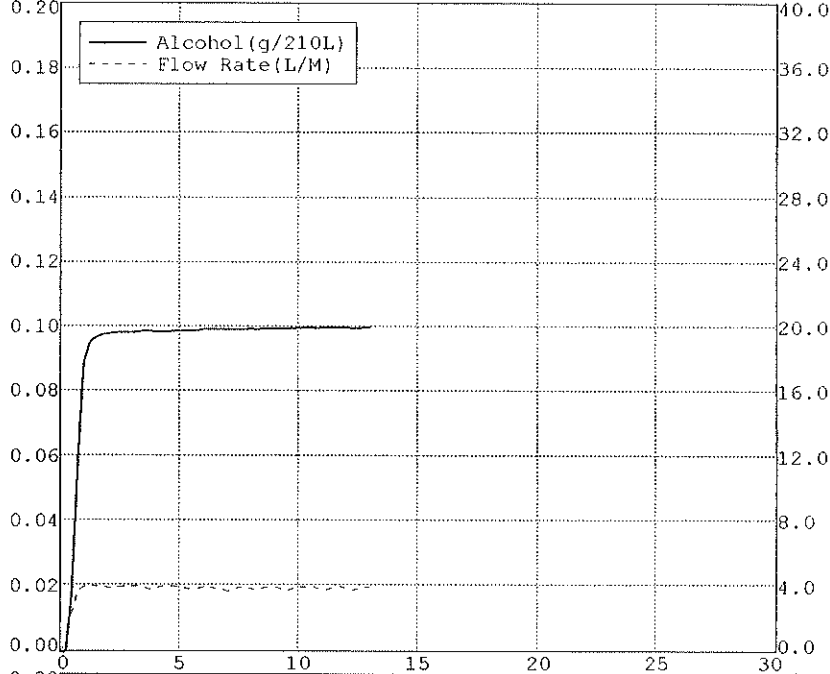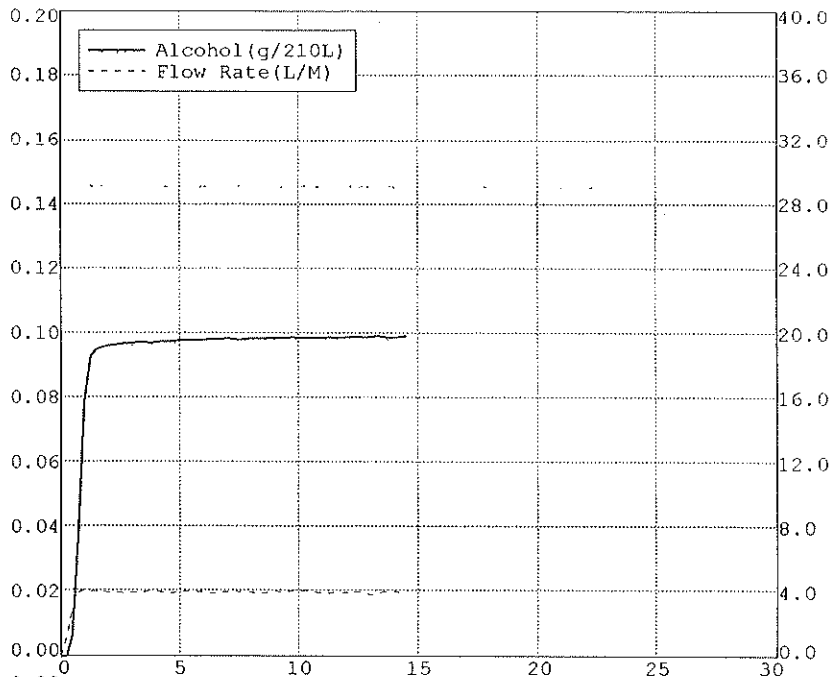

SUPERVISOR TEST

NEW HARTFORD TOWN
POLICE DEPT
DATAMASTER dmt: 127606

Date: 07/01/2020

OPERATOR NAME:
MICHAEL T KOWALSKI
Permit #: 31077
Operator Agency/Dept: NEW HARTFORD TOWN PD
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:19
INTERNAL STANDARD	VERIFIED	09:19
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:19
BLANK TEST	0.00	09:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:20
BLANK TEST	0.00	09:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:22
BLANK TEST	0.00	09:22

