

SUPERVISOR TEST

LEB




ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 01/05/2020

OPERATOR NAME:
BRETT A GRABELDINGER
Permit #: 46896
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:09
INTERNAL STANDARD	VERIFIED	01:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:10
BLANK TEST	0.00	01:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:11
BLANK TEST	0.00	01:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:12
BLANK TEST	0.00	01:13

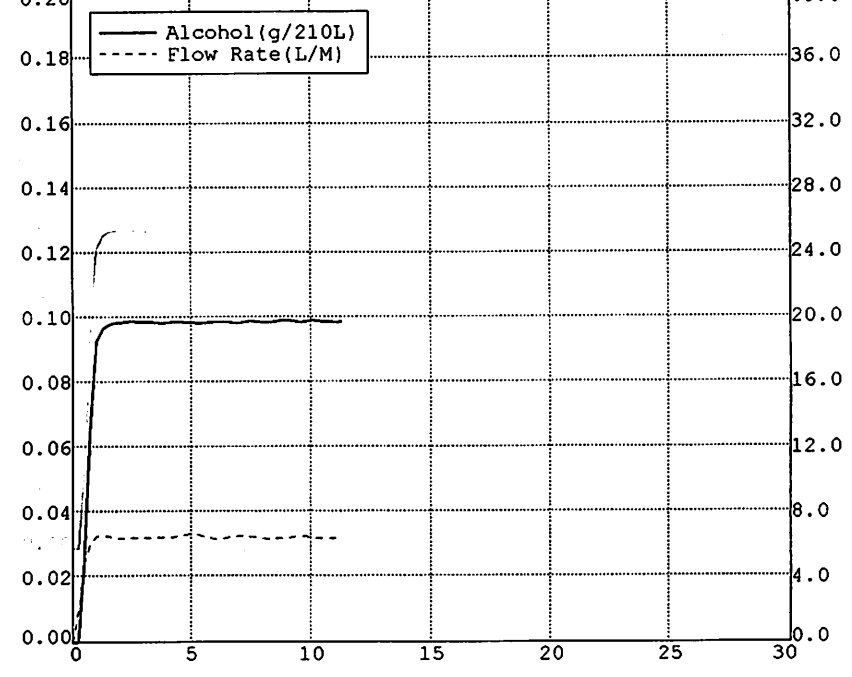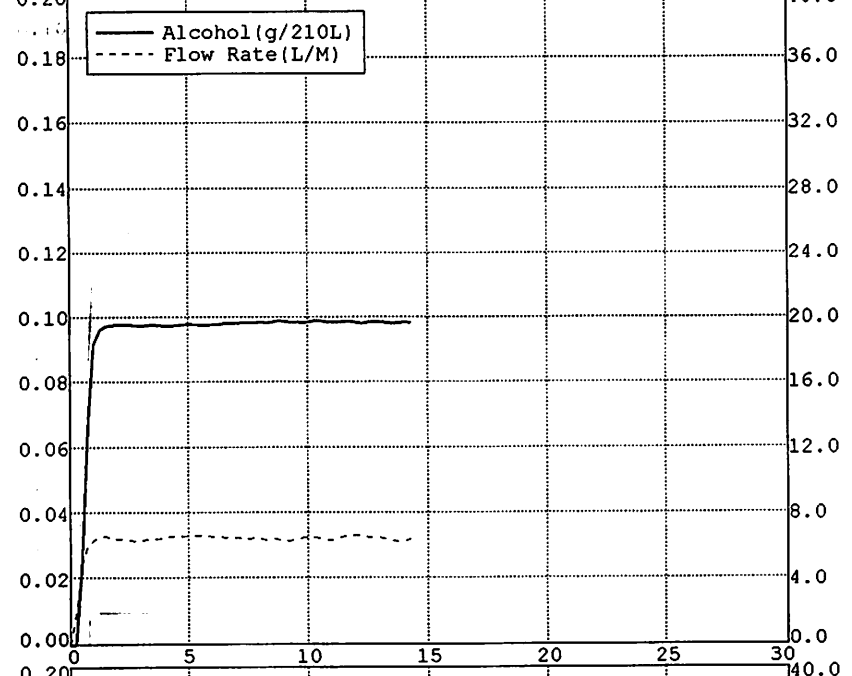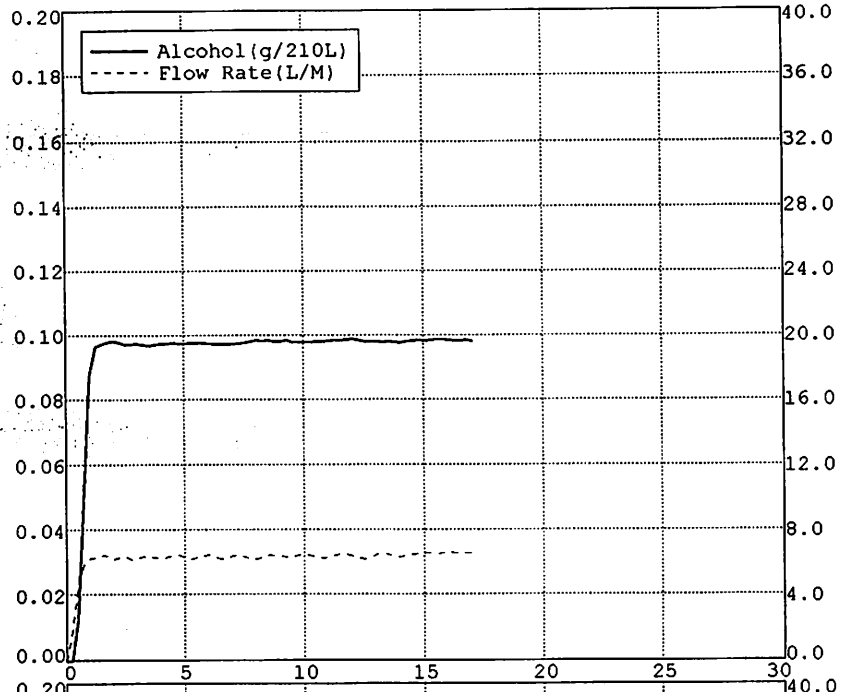

SUPERVISOR TEST

LEB

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 01/08/2020

OPERATOR NAME:
BRETT A GRABELDINGER
Permit #: 46896
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:56
INTERNAL STANDARD	VERIFIED	17:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:56
BLANK TEST	0.00	17:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:58
BLANK TEST	0.00	17:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:59
BLANK TEST	0.00	18:00

