

SUPERVISOR TEST

CFO




ONEIDA CO.  
SHERIFF'S DEPT  
DATAMASTER dmt: 123906

Date: 06/10/2020

OPERATOR NAME:  
BRETT A GRABELDINGER  
Permit #: 46896  
Operator Agency/Dept: ONEIDA CO. SO  
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:42
INTERNAL STANDARD	VERIFIED	21:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:42
BLANK TEST	0.00	21:43
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:43
BLANK TEST	0.00	21:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	21:45
BLANK TEST	0.00	21:46

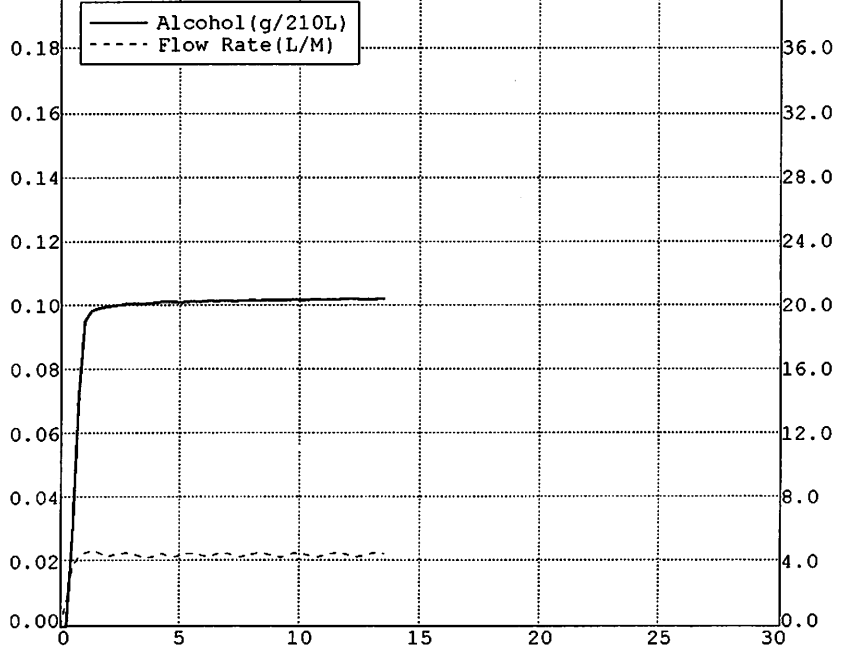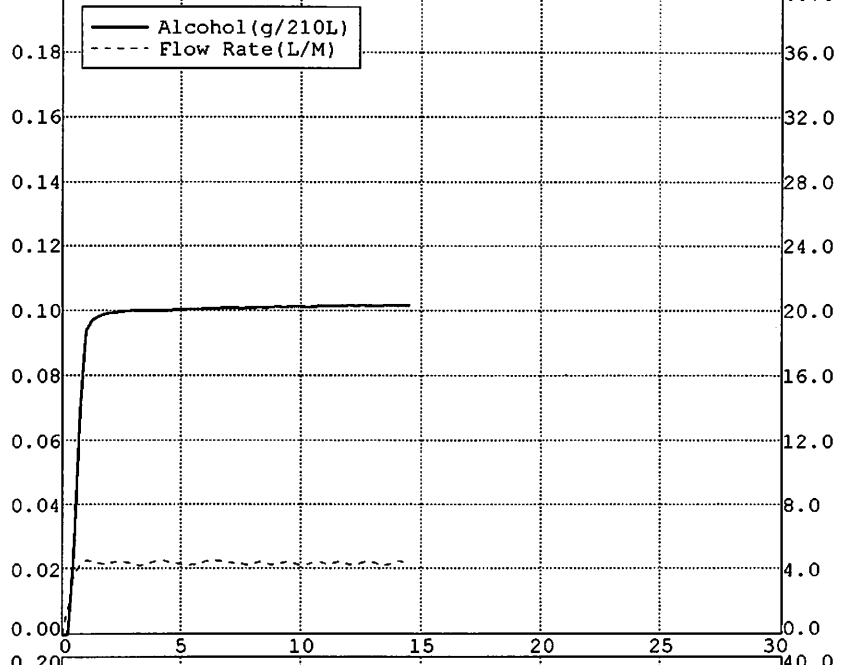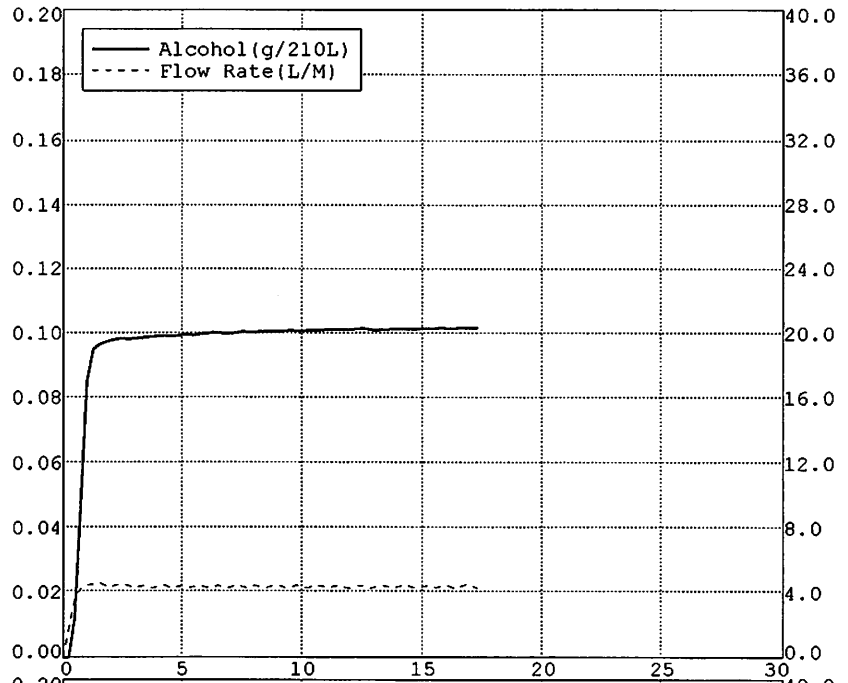

SUPERVISOR TEST

LATIC

ONEIDA CO.  
SHERIFF'S DEPT  
DATAMASTER dmt: 123906

CFD

Date: 06/18/2020

OPERATOR NAME:  
EMRAH LATIC  
Permit #: 46908  
Operator Agency/Dept: ONEIDA CO. SO  
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:43
INTERNAL STANDARD	VERIFIED	01:43
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:43
BLANK TEST	0.00	01:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:45
BLANK TEST	0.00	01:46
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:46
BLANK TEST	0.00	01:47

