

SOLUTION CHANGE




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 04/01/2019

OPERATOR NAME:
HOLLIE B KENNEDY
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:36
INTERNAL STANDARD	VERIFIED	16:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:37
BLANK TEST	0.00	16:38
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:38
BLANK TEST	0.00	16:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:39
BLANK TEST	0.00	16:40

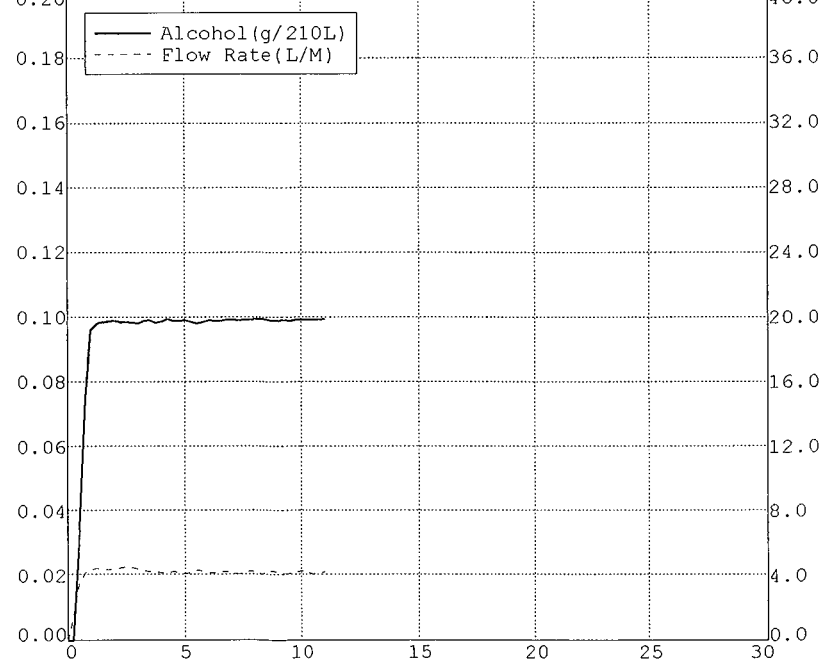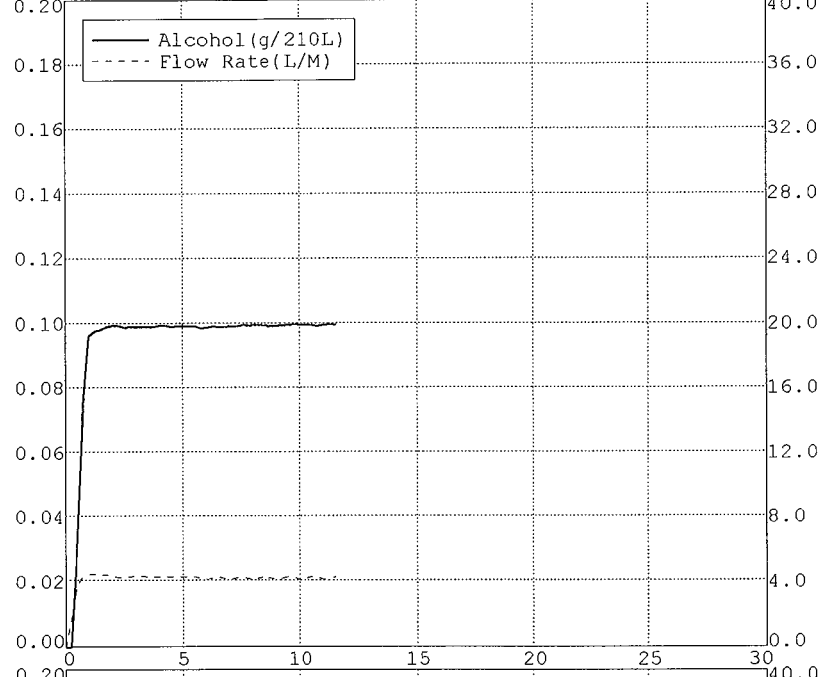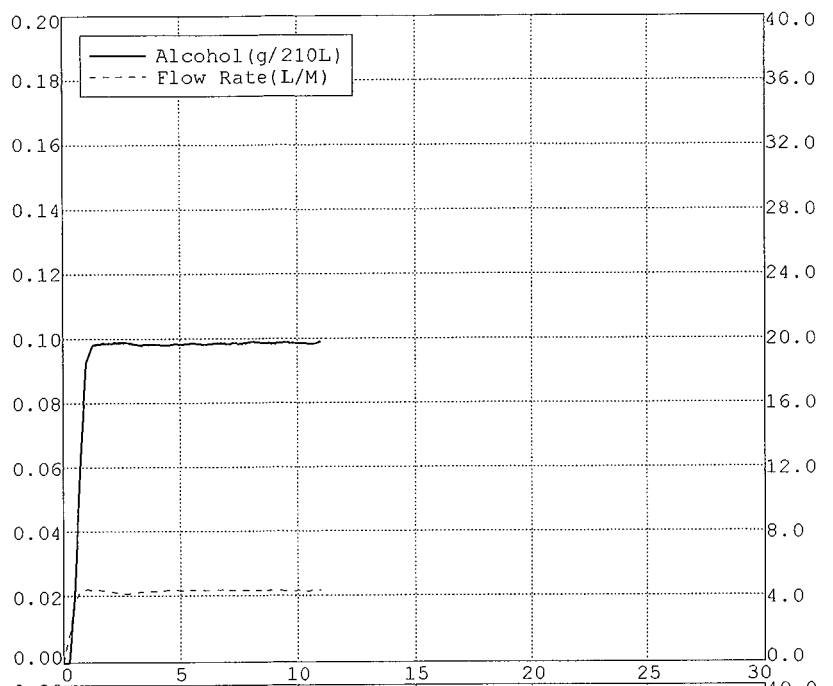

*Hollie Kennedy, Rome PD 04/01/19
Reference Standard 19030*

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 04/05/2019

OPERATOR NAME:
HOLLIE B KENNEDY
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:59
INTERNAL STANDARD	VERIFIED	19:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:59
BLANK TEST	0.00	20:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	20:00
BLANK TEST	0.00	20:01
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	20:02
BLANK TEST	0.00	20:02

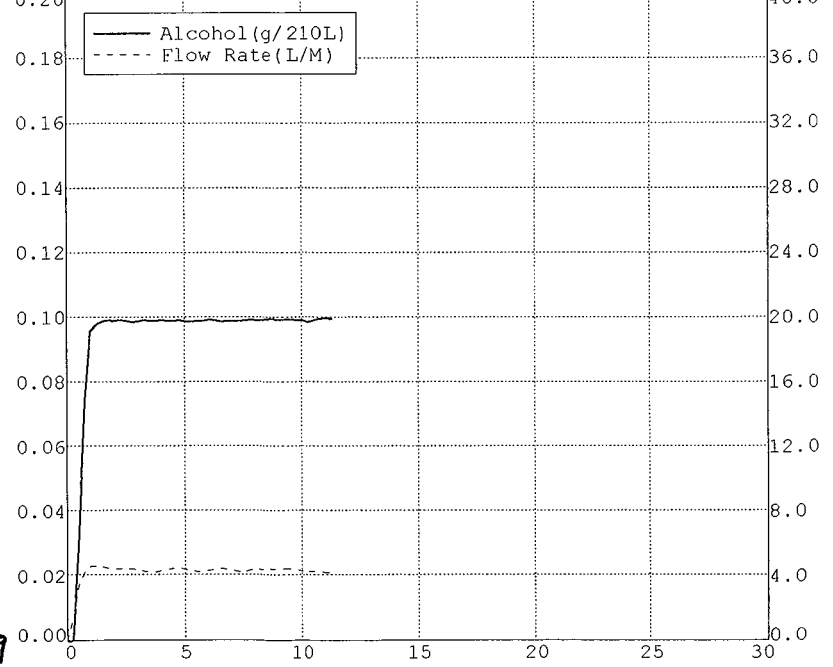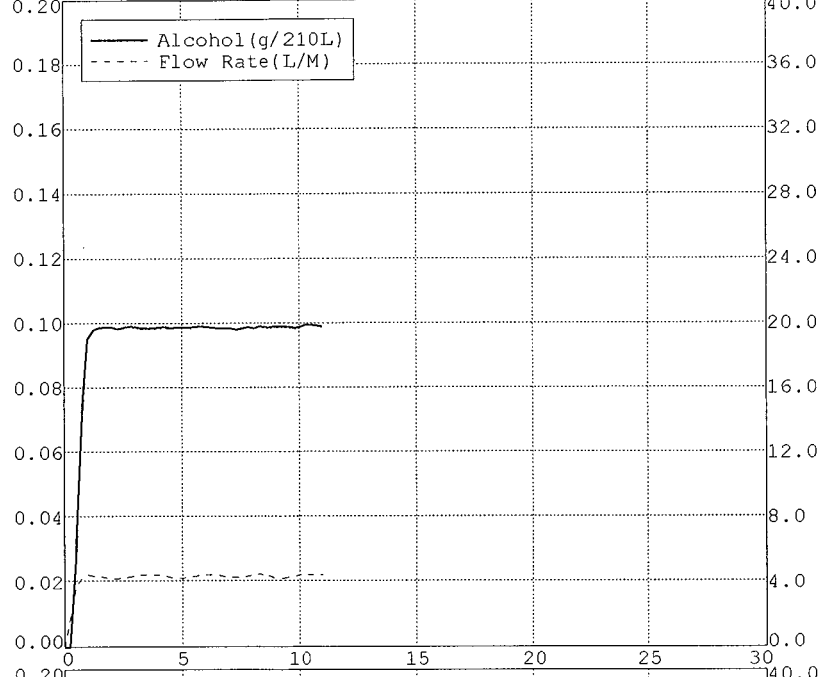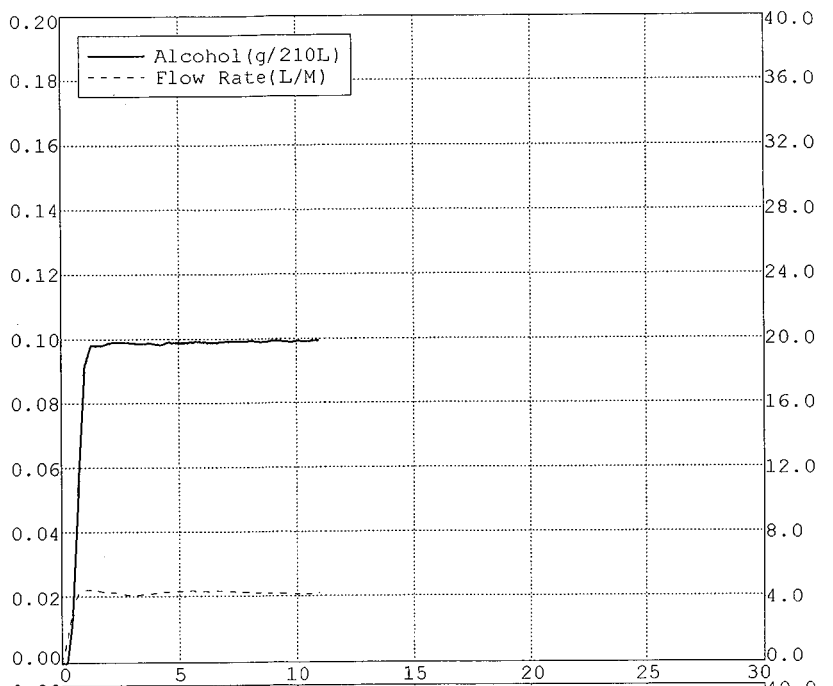

Hollie Kennedy Rome PD 04/05/19
Hollie Kennedy 10/02

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 04/12/2019

OPERATOR NAME:
HOLLIE B KENNEDY
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:28
INTERNAL STANDARD	VERIFIED	15:28
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:29
BLANK TEST	0.00	15:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:30
BLANK TEST	0.00	15:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:31
BLANK TEST	0.00	15:32

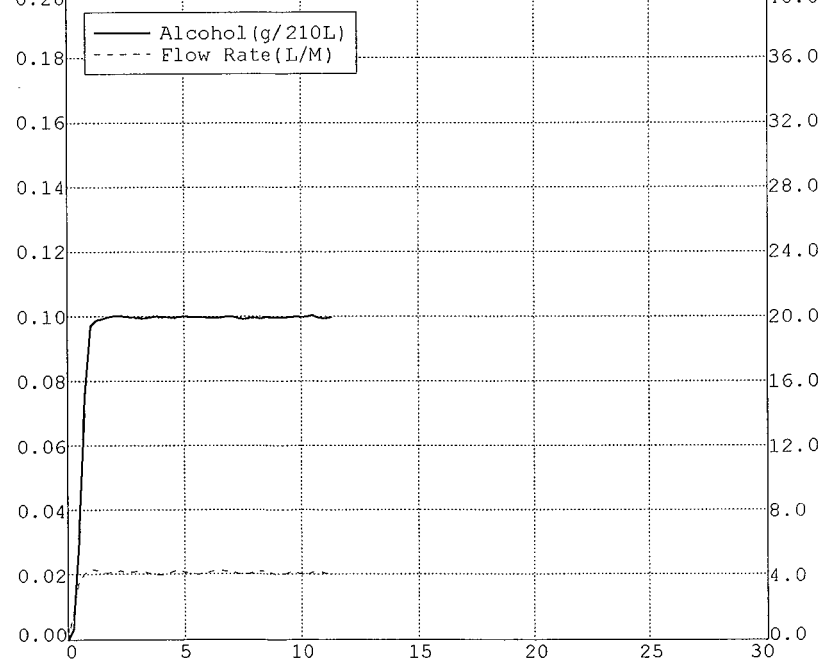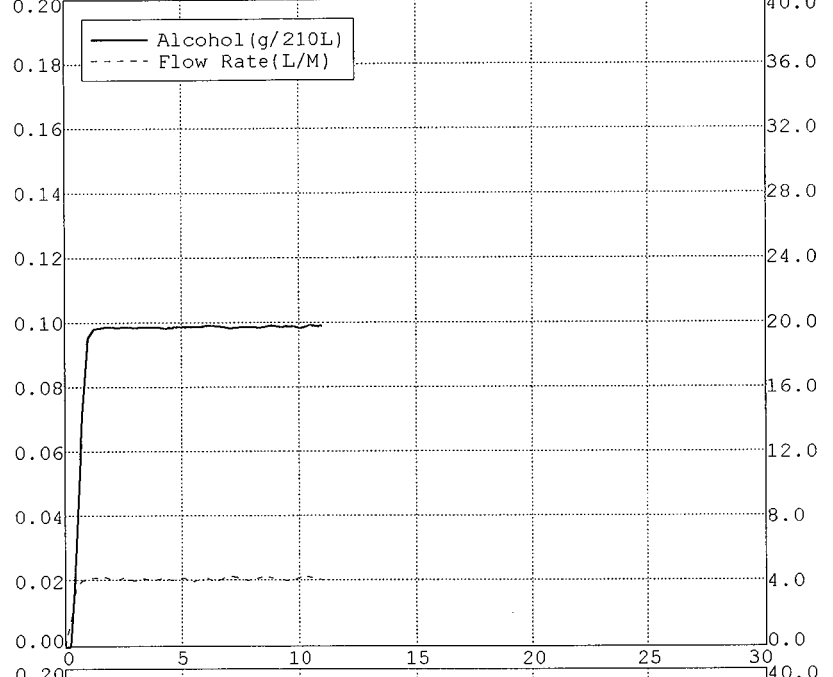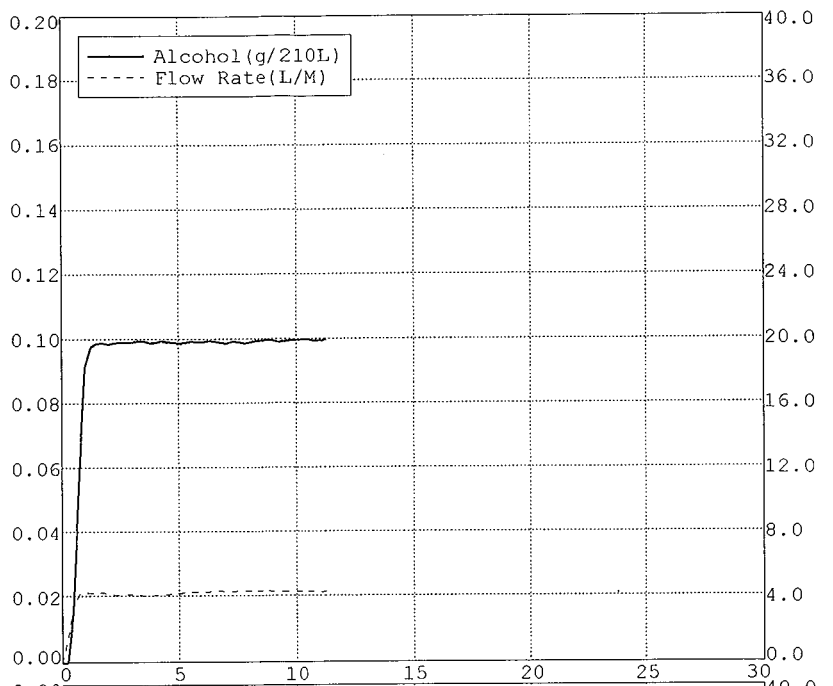

Hollie B Kennedy Rome CPD 04/12/19
1885

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 04/20/2019

OPERATOR NAME:
HOLLIE B KENNEDY
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:16
INTERNAL STANDARD	VERIFIED	16:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:17
BLANK TEST	0.00	16:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:18
BLANK TEST	0.00	16:19
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:19
BLANK TEST	0.00	16:20

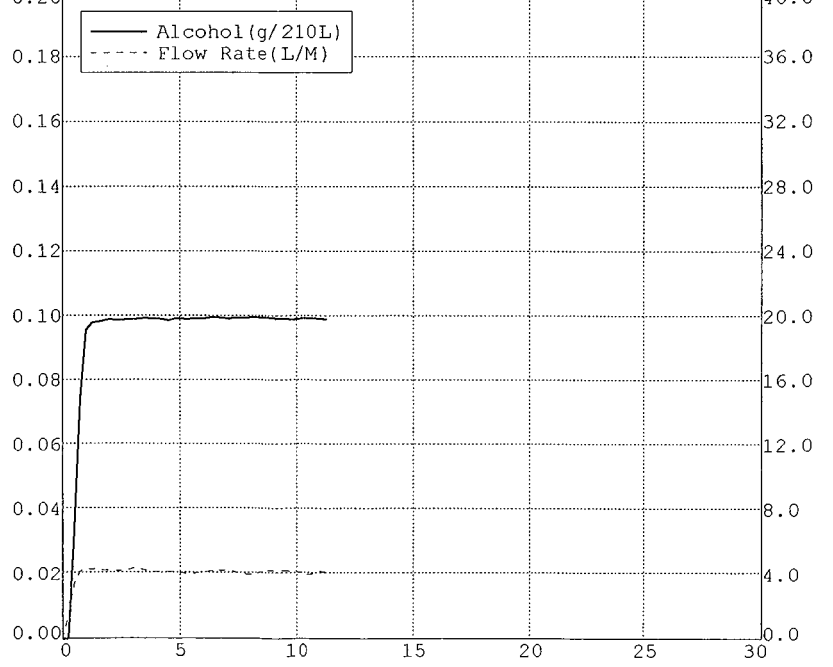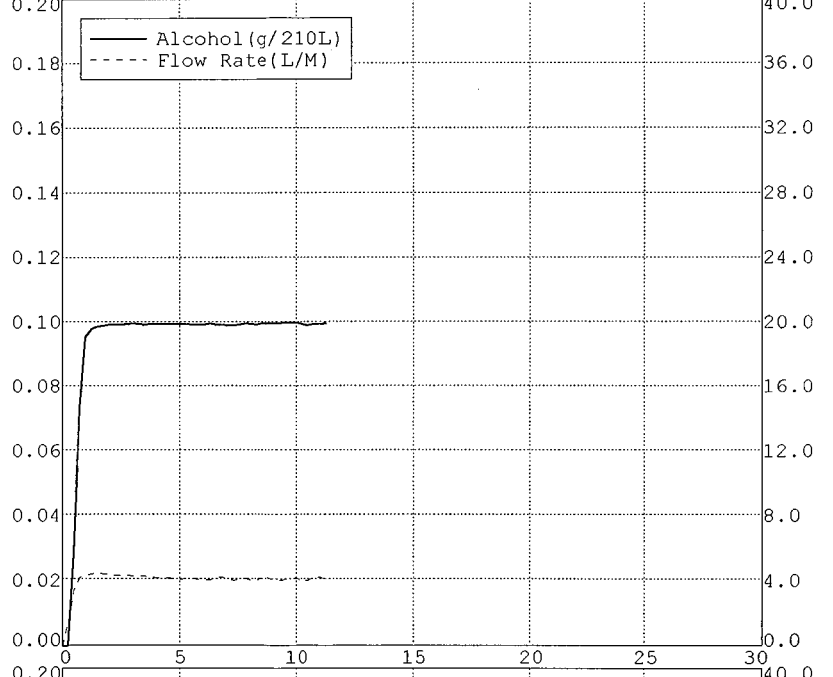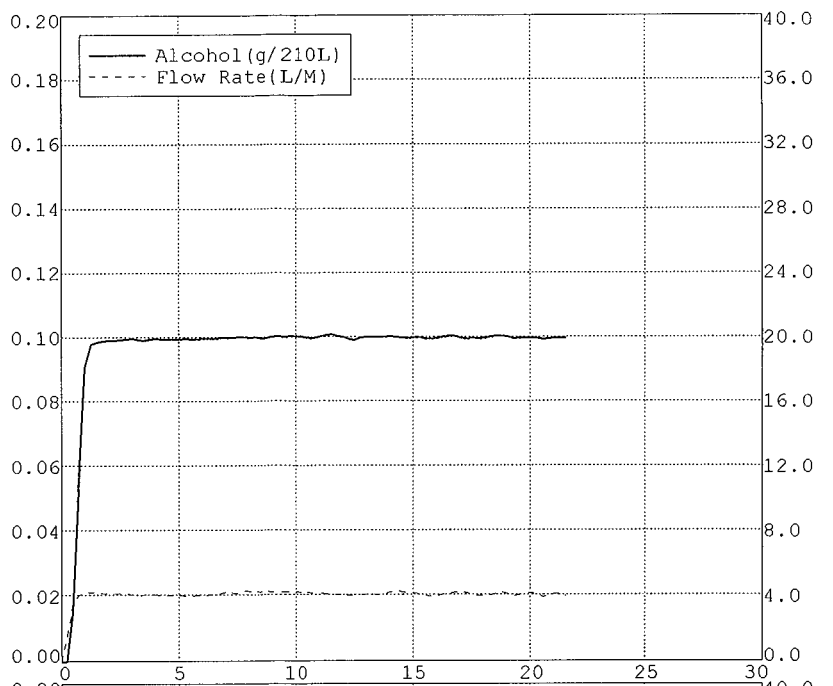

Hollie B Kennedy Rome PD 4/20/19
Shirley 1005

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 04/25/2019

OPERATOR NAME:
HOLLIE B KENNEDY
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:36
INTERNAL STANDARD	VERIFIED	22:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	22:36
BLANK TEST	0.00	22:37
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	22:38
BLANK TEST	0.00	22:38
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	22:39
BLANK TEST	0.00	22:40

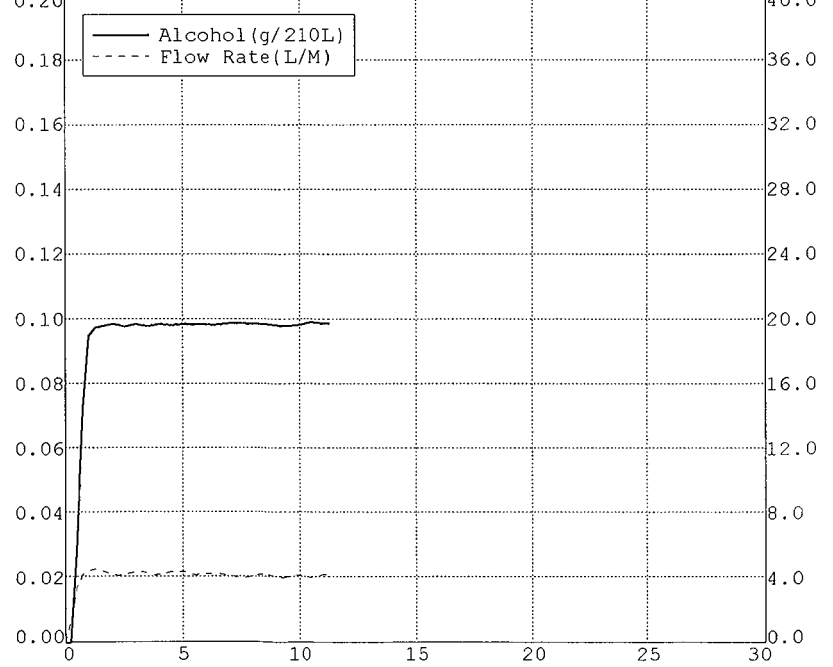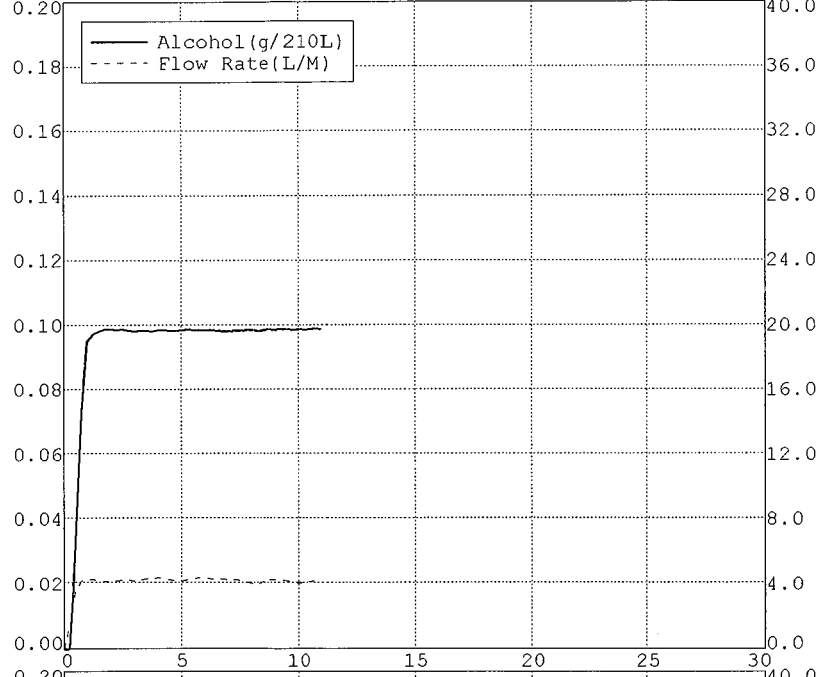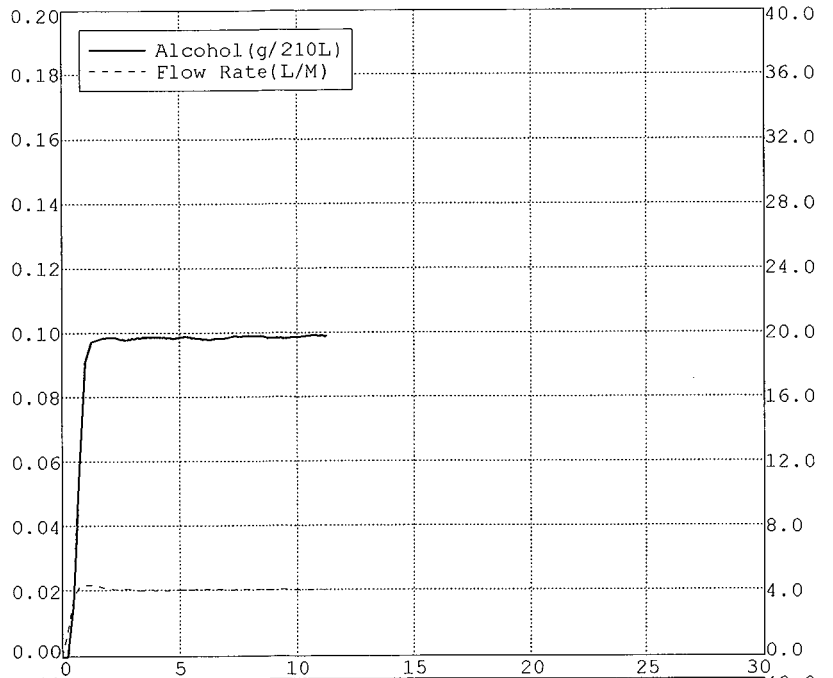

Hollie Kennedy Rome PD 04/25/19
Hollie Kennedy 1005