

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 04/10/2020

OPERATOR NAME:
HOLLIE B SILVERMAN
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:23
INTERNAL STANDARD	VERIFIED	18:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:24
BLANK TEST	0.00	18:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	18:25
BLANK TEST	0.00	18:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:26
BLANK TEST	0.00	18:27

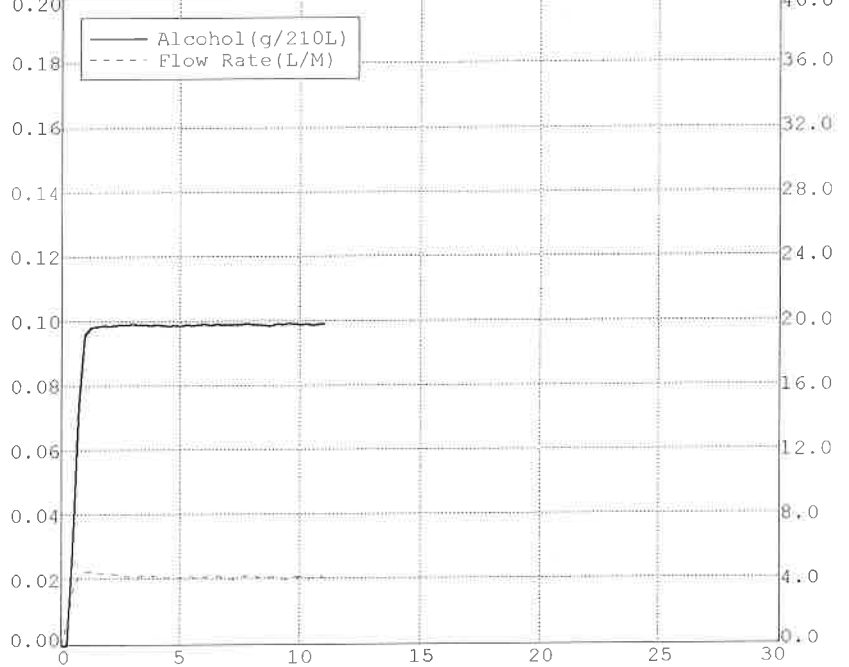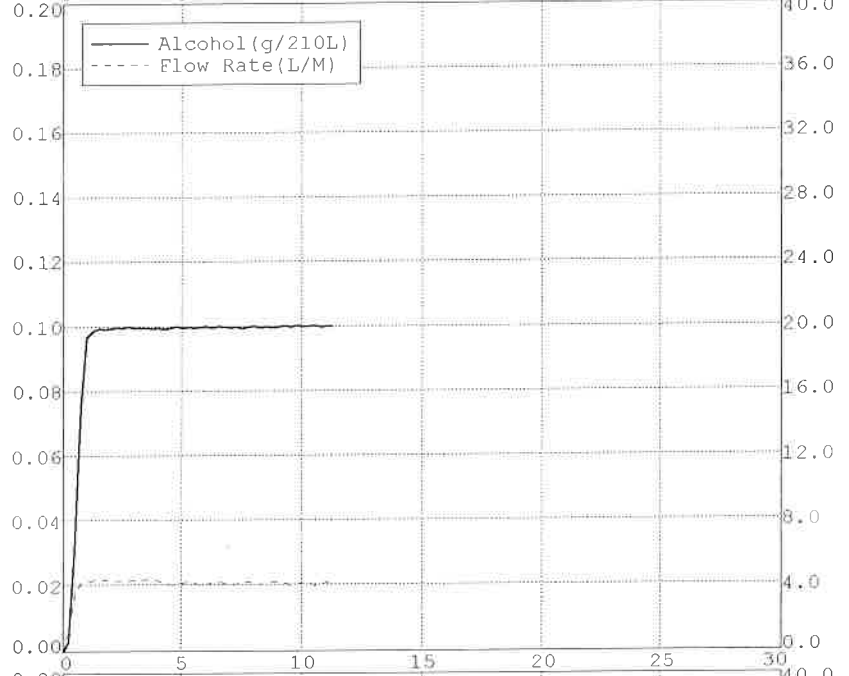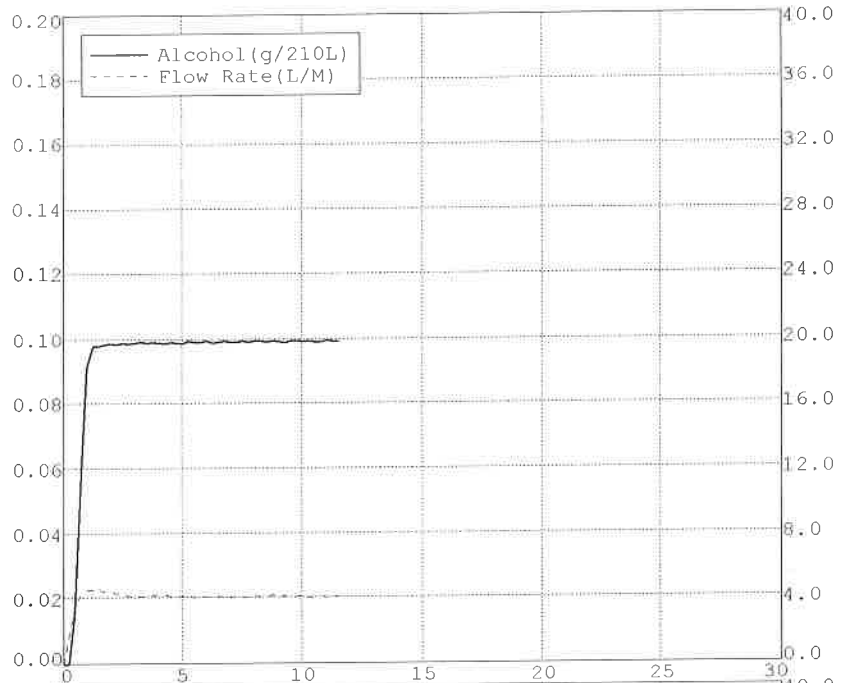

Hollie B Silverman Rome PD 04/10/2020
Hollie B Silverman 10805