

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 06/07/2020

OPERATOR NAME:
HOLLIE B SILVERMAN
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:08
INTERNAL STANDARD	VERIFIED	12:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:09
BLANK TEST	0.00	12:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:10
BLANK TEST	0.00	12:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:11
BLANK TEST	0.00	12:12

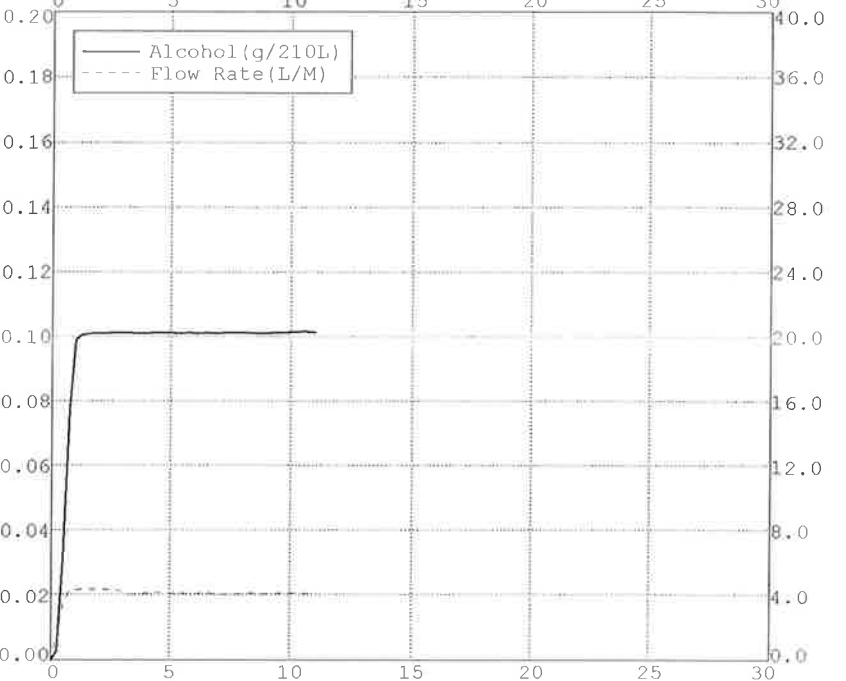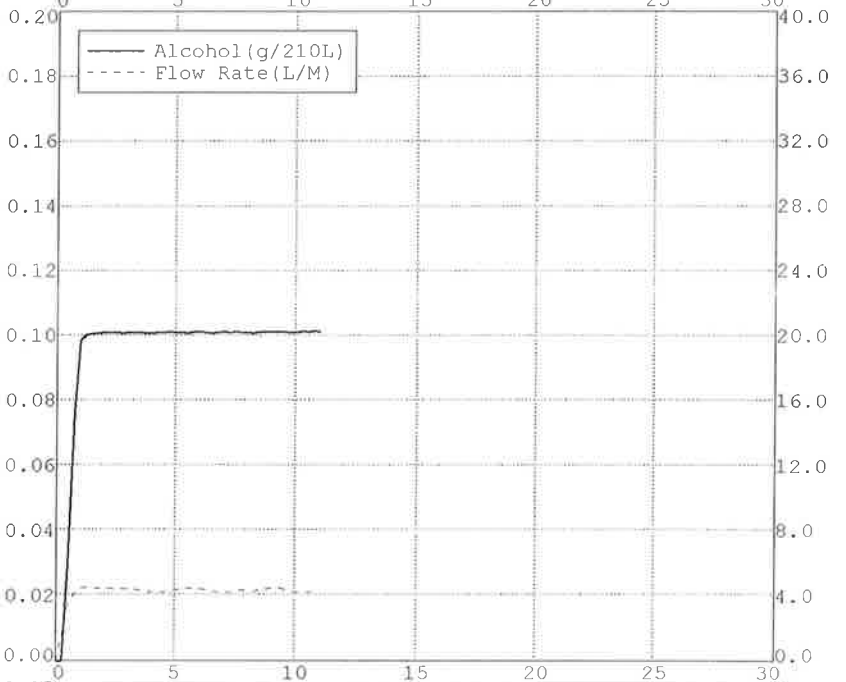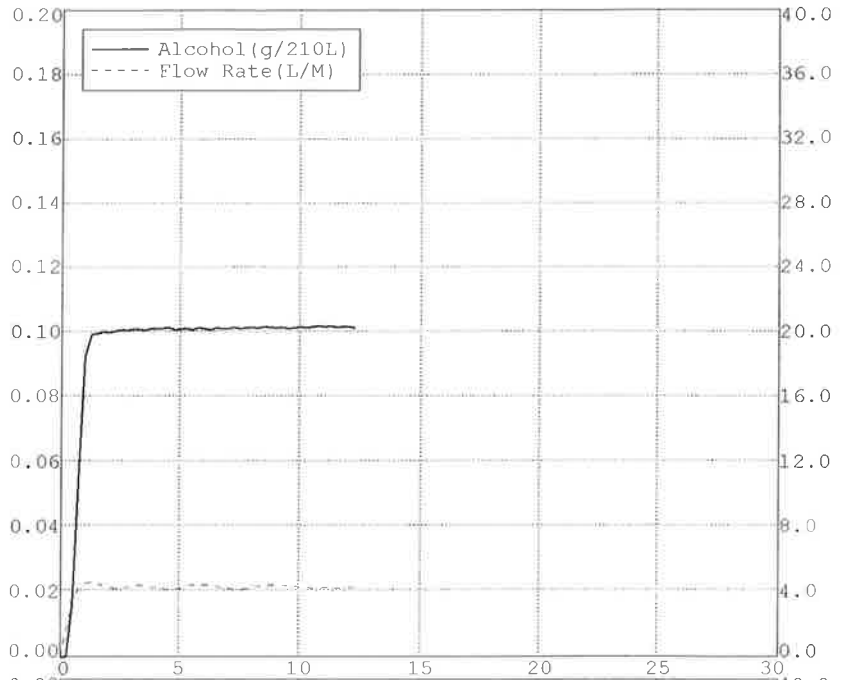

Hollie B Silverman, Rome PD
Hollie B Silverman 10/15

06/07/2020