

SOLUTION CHANGE

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308




Date: 06/01/2020

RM)
20-18676

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 355

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:58
INTERNAL STANDARD	VERIFIED	13:58
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	13:59
BLANK TEST	0.00	13:59
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	14:00
BLANK TEST	0.00	14:01
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	14:01
BLANK TEST	0.00	14:02

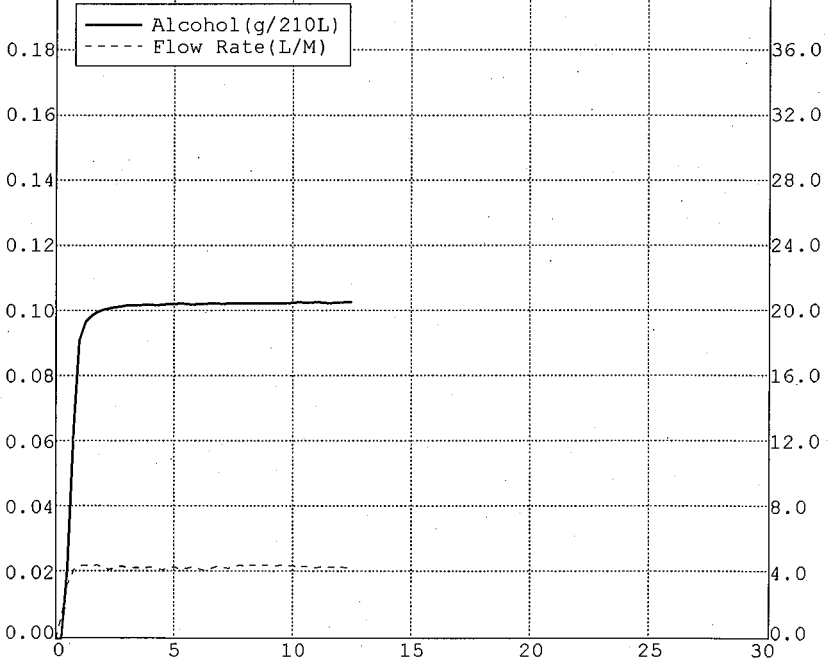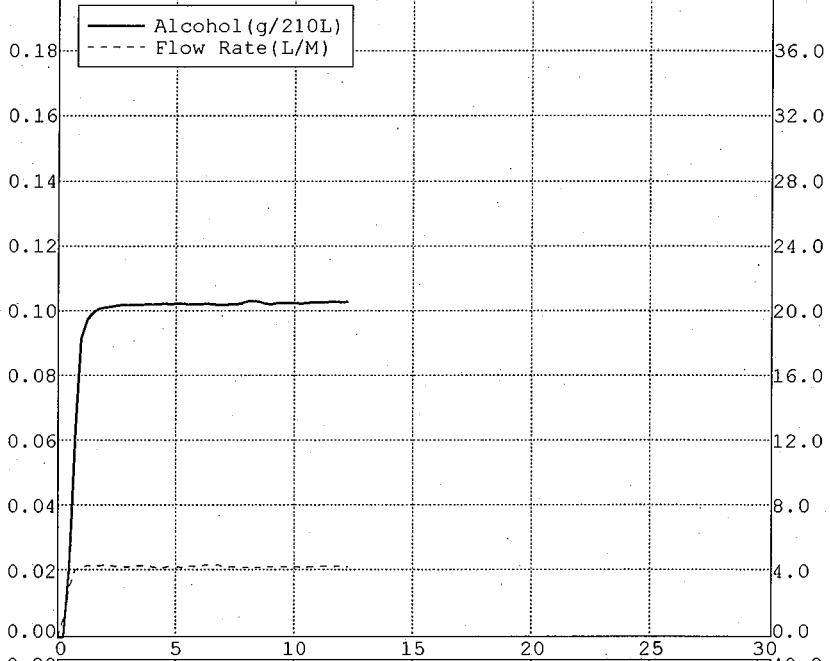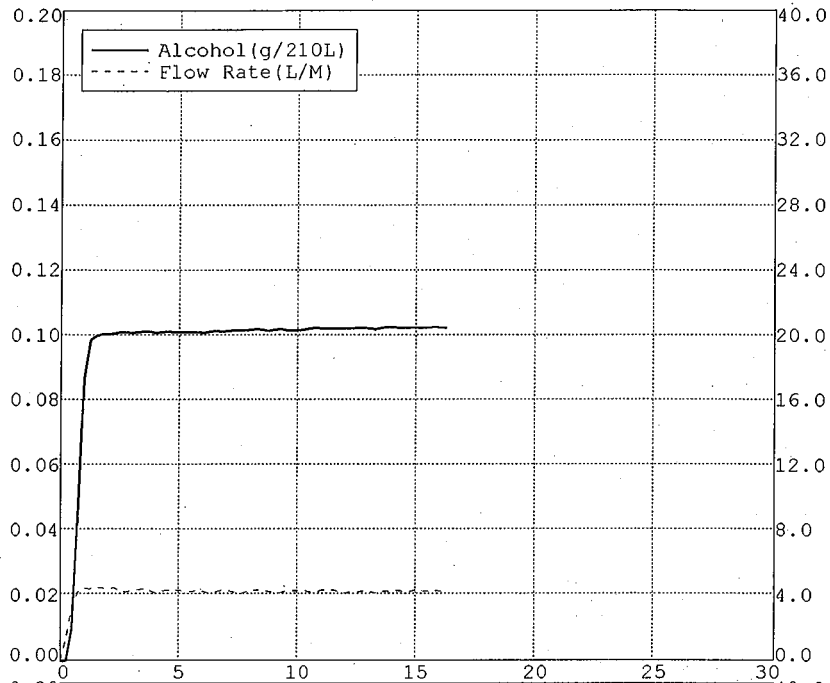

SOLUTION CHANGE

UTICA CITY
 POLICE DEPT
 DATAMASTER dmt: 100282

Date: 06/01/2020

RMJ
20-18676

OPERATOR NAME:
 MICHAEL J CLIVE
 Permit #: 36682
 Operator Agency/Dept: UTICA CITY PD
 Reference Standard #: 282

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:57
INTERNAL STANDARD	VERIFIED	13:57
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	13:57
BLANK TEST	0.00	13:58
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	13:58
BLANK TEST	0.00	13:59
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	13:59
BLANK TEST	0.00	14:00

