

SUPERVISOR TEST




UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308

Date: 11/26/2019

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 19180

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 13:28 |
| INTERNAL STANDARD | VERIFIED | 13:28 |
| REFERENCE STANDARD TEMP | 34.02c | |
| REFERENCE STANDARD | 0.10 | 13:29 |
| BLANK TEST | 0.00 | 13:30 |
| REFERENCE STANDARD TEMP | 34.02c | |
| REFERENCE STANDARD | 0.10 | 13:30 |
| BLANK TEST | 0.00 | 13:31 |
| REFERENCE STANDARD TEMP | 34.02c | |
| REFERENCE STANDARD | 0.10 | 13:31 |
| BLANK TEST | 0.00 | 13:32 |

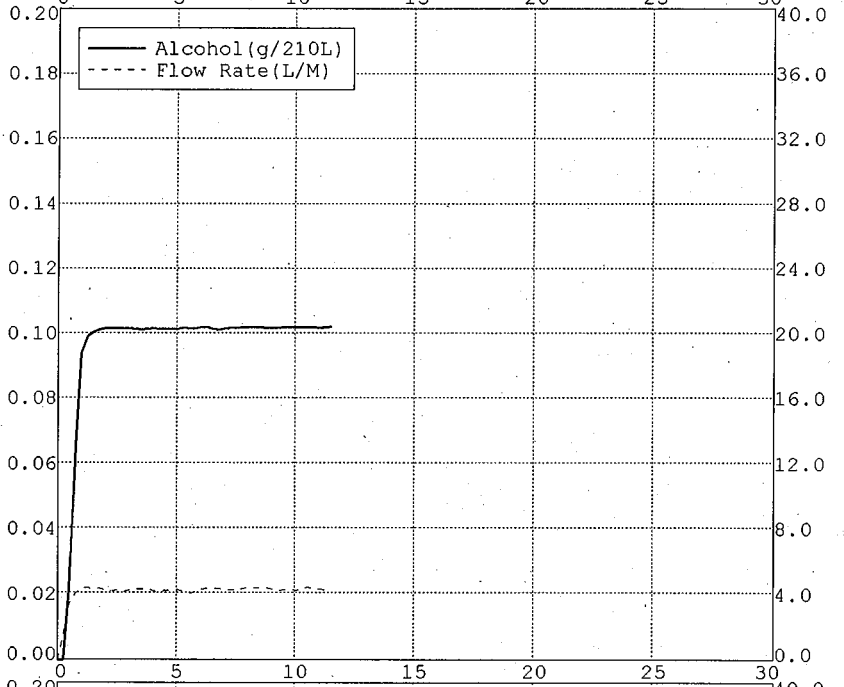

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282

Date: 11/26/2019

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 19180

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 13:27 |
| INTERNAL STANDARD | VERIFIED | 13:27 |
| REFERENCE STANDARD TEMP | 33.99c | |
| REFERENCE STANDARD | 0.09 | 13:28 |
| BLANK TEST | 0.00 | 13:29 |
| REFERENCE STANDARD TEMP | 33.99c | |
| REFERENCE STANDARD | 0.09 | 13:29 |
| BLANK TEST | 0.00 | 13:30 |
| REFERENCE STANDARD TEMP | 33.99c | |
| REFERENCE STANDARD | 0.10 | 13:30 |
| BLANK TEST | 0.00 | 13:31 |

