

SUPERVISOR TEST

UTICA CITY  
POLICE DEPT  
DATAMASTER dmt: 107308




Date: 06/16/2020

*RMJ*  
*20-21218*

OPERATOR NAME:  
MICHAEL J CLIVE  
Permit #: 36682  
Operator Agency/Dept: UTICA CITY PD  
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:54
INTERNAL STANDARD	VERIFIED	12:54
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:54
BLANK TEST	0.00	12:55
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:56
BLANK TEST	0.00	12:56
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:57
BLANK TEST	0.00	12:57

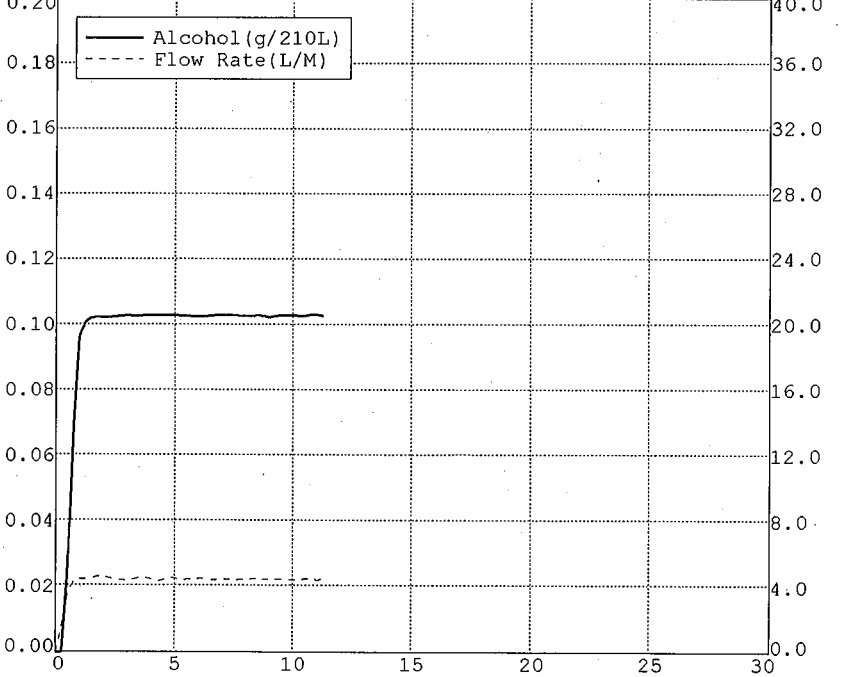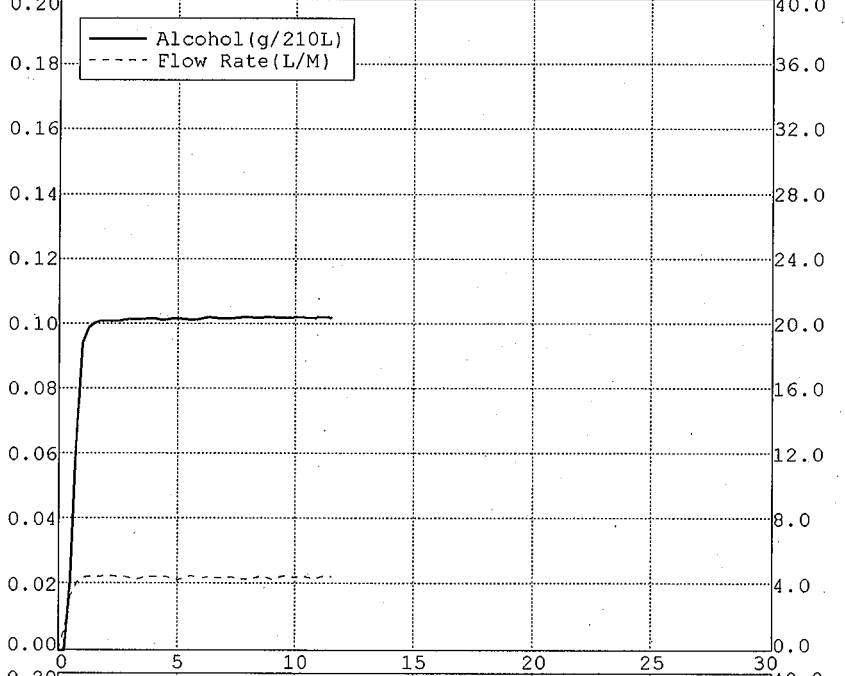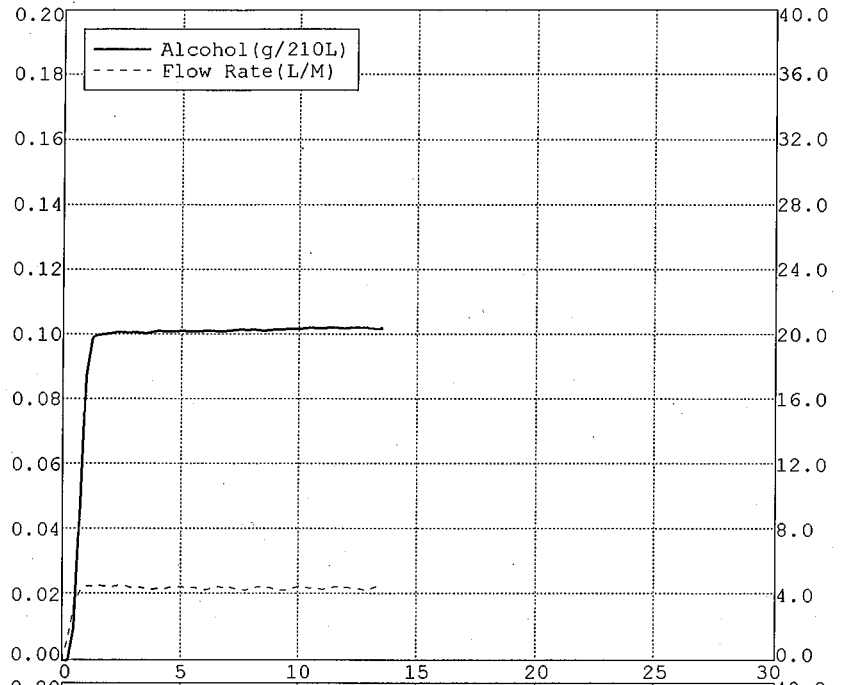

SUPERVISOR TEST

UTICA CITY  
POLICE DEPT  
DATAMASTER dmt: 100282

Date: 06/16/2020

*RM*  
*20-21218*

OPERATOR NAME:  
MICHAEL J CLIVE  
Permit #: 36682  
Operator Agency/Dept: UTICA CITY PD  
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:42
INTERNAL STANDARD	VERIFIED	12:42
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	12:43
BLANK TEST	0.00	12:43
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	12:44
BLANK TEST	0.00	12:45
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	12:45
BLANK TEST	0.00	12:46

