

SUPERVISOR TEST

UTICA CITY  
 POLICE DEPT  
 DATAMASTER dmt: 100282




Date: 03/17/2020

*RM*  
*20-9038*

OPERATOR NAME:  
 MICHAEL J CLIVE  
 Permit #: 36682  
 Operator Agency/Dept: UTICA CITY PD  
 Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:17
INTERNAL STANDARD	VERIFIED	12:17
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	12:18
BLANK TEST	0.00	12:18
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	12:19
BLANK TEST	0.00	12:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:20
BLANK TEST	0.00	12:21

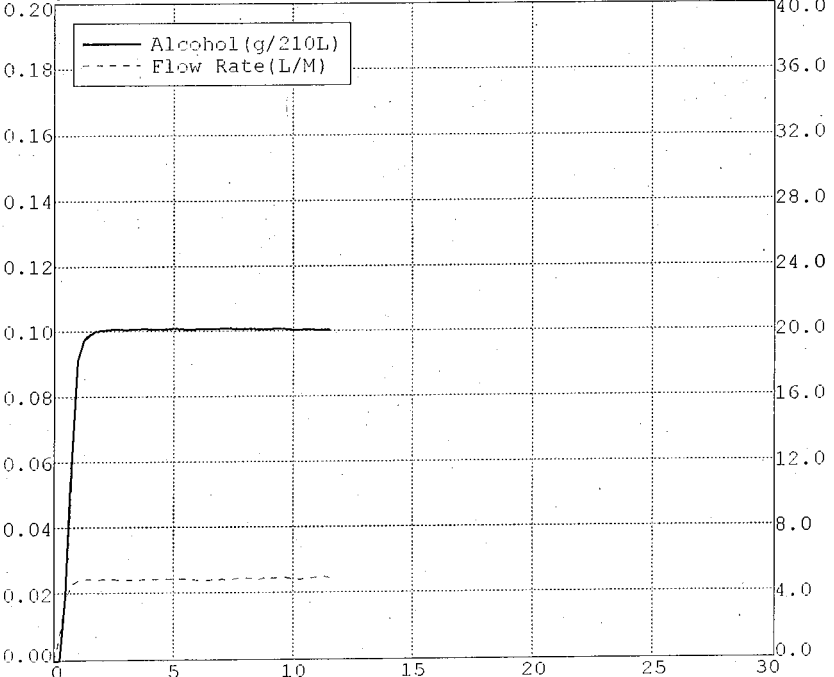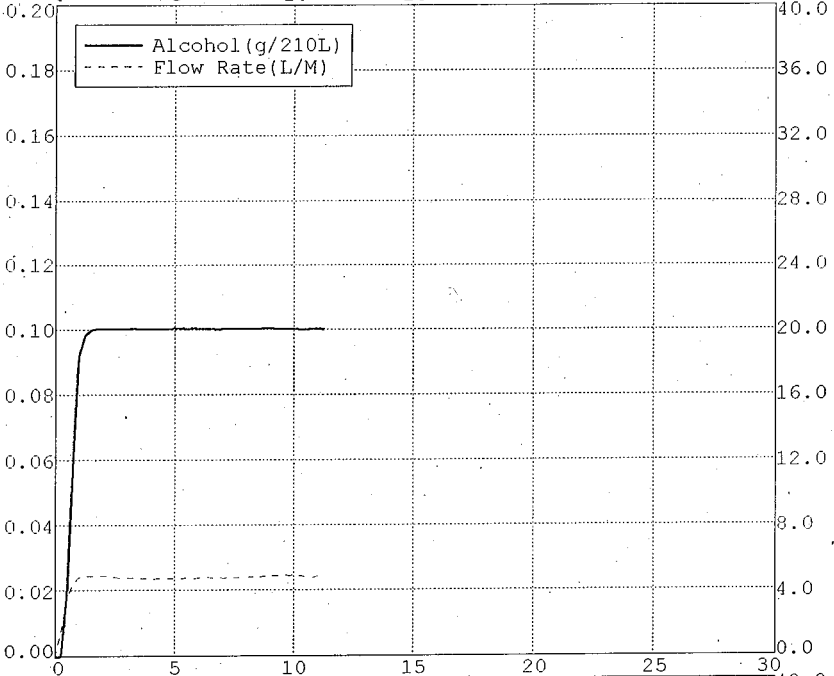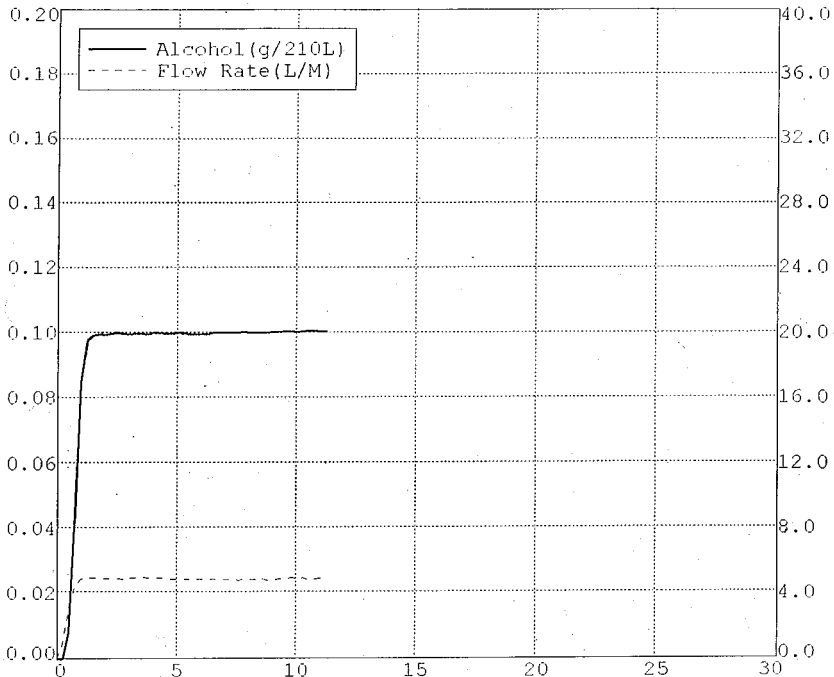

SUPERVISOR TEST

UTICA CITY  
POLICE DEPT  
DATAMASTER dmt: 107308

Date: 03/17/2020

*RMS*  
*20-9038*

OPERATOR NAME:  
MICHAEL J CLIVE  
Permit #: 36682  
Operator Agency/Dept: UTICA CITY PD  
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:47
INTERNAL STANDARD	VERIFIED	12:47
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:48
BLANK TEST	0.00	12:48
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:49
BLANK TEST	0.00	12:50
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:50
BLANK TEST	0.00	12:51

