

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308




RMJ
20-2/25

Date: 01/23/2020

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:26
INTERNAL STANDARD	VERIFIED	09:26
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	09:27
BLANK TEST	0.00	09:28
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	09:28
BLANK TEST	0.00	09:29
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	09:29
BLANK TEST	0.00	09:30

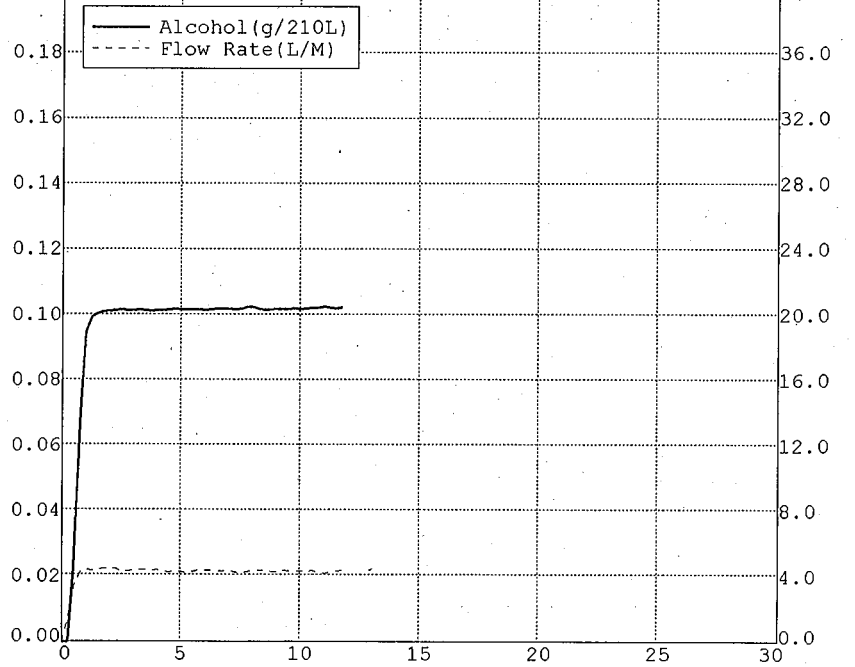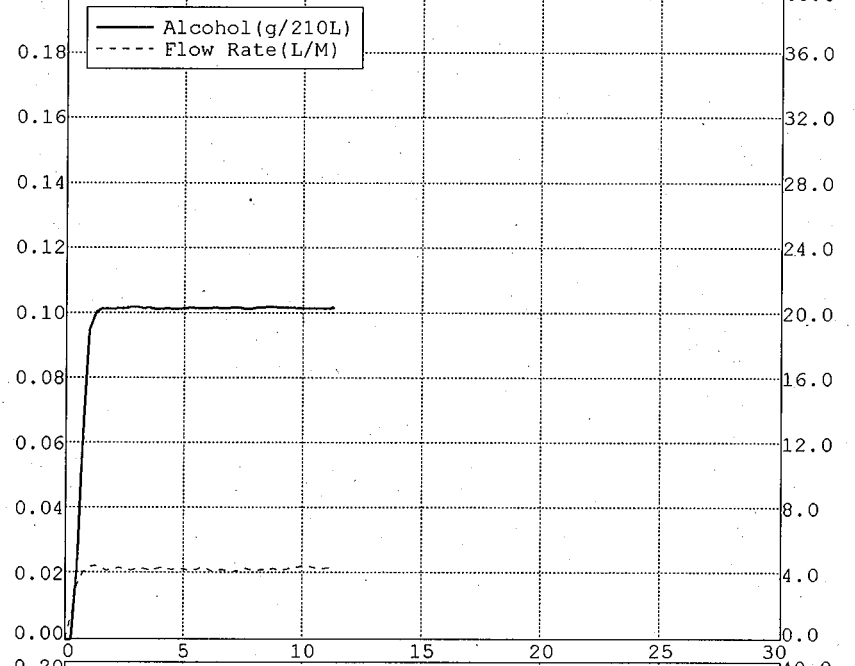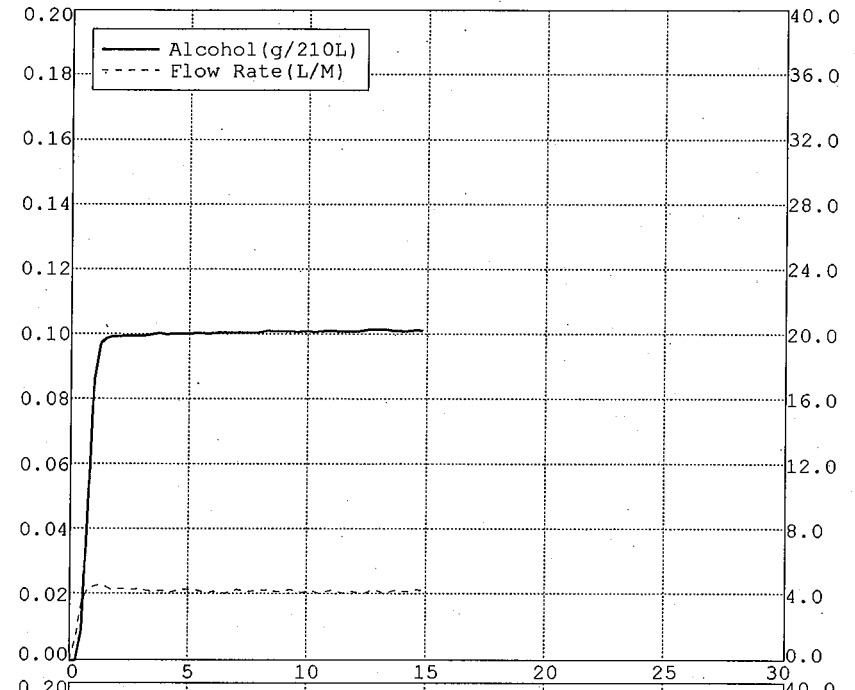

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282

Date: 01/23/2020

RM
20-21/25

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:12
INTERNAL STANDARD	VERIFIED	09:12
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	09:13
BLANK TEST	0.00	09:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:14
BLANK TEST	0.00	09:15
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	09:15
BLANK TEST	0.00	09:16

