

SUPERVISOR TEST




-----  
WHITESTOWN TOWN  
POLICE DEPT.  
DATAMASTER dmt: 100231  
-----

ate: 11/24/2019

OPERATOR NAME:  
D J HUMPHRIES II  
Permit #: 40440  
Operator Agency/Dept: WHITESTOWN TOWN PD  
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:58
INTERNAL STANDARD	VERIFIED	14:58
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	14:59
BLANK TEST	0.00	14:59
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	15:00
BLANK TEST	0.00	15:01
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	15:01
BLANK TEST	0.00	15:02

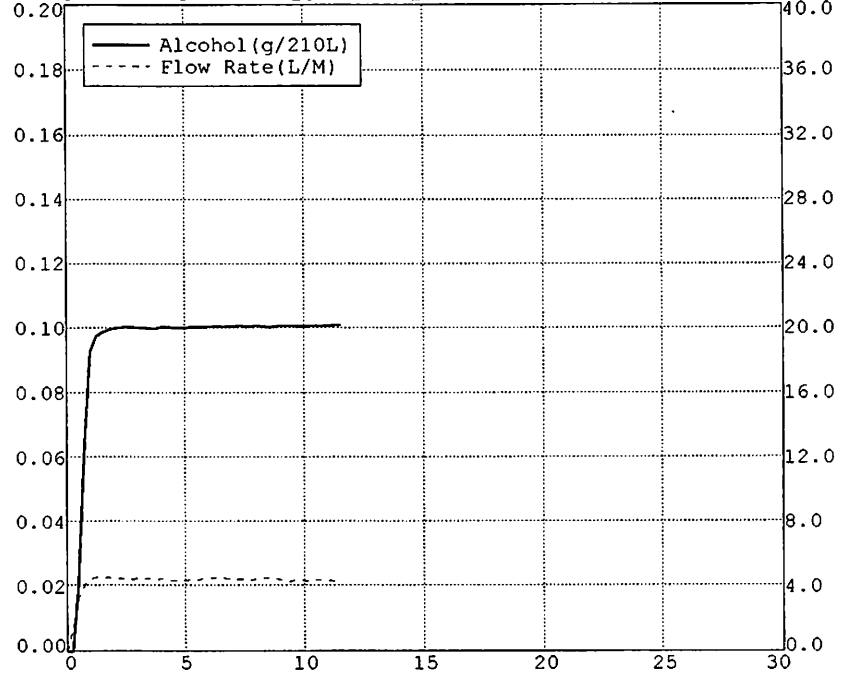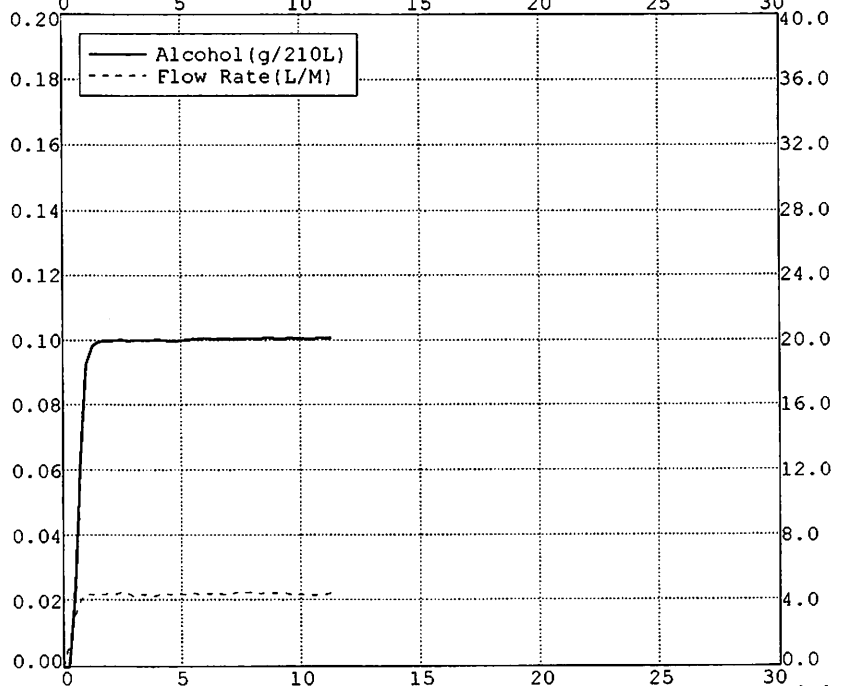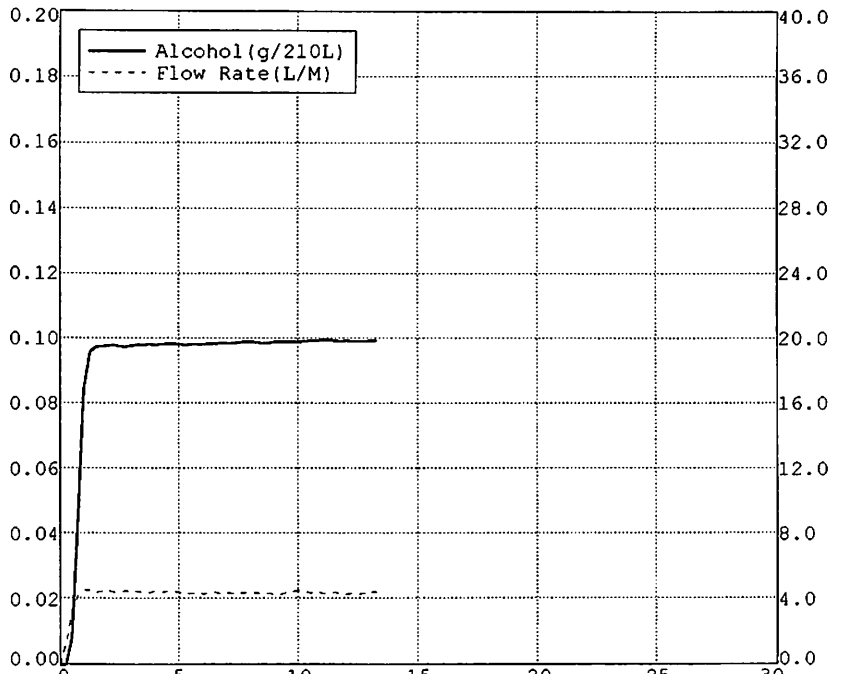

SUPERVISOR TEST

-----  
WHITESTOWN TOWN  
POLICE DEPT.  
DATAMASTER dmt: 100231  
-----

Date: 11/05/2019

OPERATOR NAME:  
D J HUMPHRIES II  
Permit #: 40440  
Operator Agency/Dept: TOWN OF WHITESTOWN PD  
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:14
INTERNAL STANDARD	VERIFIED	21:14
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	21:14
BLANK TEST	0.00	21:15
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	21:15
BLANK TEST	0.00	21:16
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	21:17
BLANK TEST	0.00	21:18

